



## testo 770 - Clamp meter

0590 7701

0590 7702

0590 7703

0590 3770

Instruction manual



# 1 Contents

|          |                                                                   |           |
|----------|-------------------------------------------------------------------|-----------|
| <b>1</b> | <b>Contents .....</b>                                             | <b>2</b>  |
| <b>2</b> | <b>Observe prior to use! .....</b>                                | <b>4</b>  |
| <b>3</b> | <b>Safety instructions .....</b>                                  | <b>4</b>  |
| <b>4</b> | <b>Intended use .....</b>                                         | <b>6</b>  |
| <b>5</b> | <b>Overview .....</b>                                             | <b>7</b>  |
| 5.1      | Display and control elements .....                                | 7         |
| 5.2      | LC display.....                                                   | 8         |
| 5.3      | Control key functions .....                                       | 9         |
| 5.4      | Rotary switch functions.....                                      | 9         |
| 5.5      | Further functions .....                                           | 10        |
| 5.5.1    | Bluetooth® (testo 770-3 only) .....                               | 10        |
| 5.5.2    | HOLD .....                                                        | 10        |
| 5.5.3    | MAX/MIN/AVG .....                                                 | 11        |
| 5.6      | Explanation of icons.....                                         | 12        |
| <b>6</b> | <b>Operating the instrument .....</b>                             | <b>13</b> |
| 6.1      | Switching the instrument on .....                                 | 14        |
| 6.2      | Switching the background illumination on/off .....                | 14        |
| 6.3      | Switching the instrument off (automatically/manually)<br>.....    | 14        |
| 6.3.1    | Automatically .....                                               | 14        |
| 6.3.2    | Manually .....                                                    | 14        |
| 6.4      | Using testo 770-3 with testo Smart App.....                       | 15        |
| 6.4.1    | Establishing Bluetooth® connection (testo 770-3)<br>.....         | 15        |
| 6.4.2    | Transmitting readings .....                                       | 15        |
| 6.4.3    | Overview of the App operating controls.....                       | 16        |
| <b>7</b> | <b>Carrying out a measurement.....</b>                            | <b>17</b> |
| 7.1      | Preparing for measurement .....                                   | 17        |
| 7.2      | Current measurement.....                                          | 17        |
| 7.2.1    | Measuring A AC or A DC .....                                      | 18        |
| 7.2.1.1  | Automatic measuring mode .....                                    | 18        |
| 7.2.1.2  | Manual measuring mode.....                                        | 18        |
| 7.2.2    | Measuring $\mu$ A AC or $\mu$ A DC (testo 770-2/-3 only)<br>..... | 19        |
| 7.2.2.1  | Automatic measuring mode .....                                    | 19        |
| 7.2.2.2  | Manual measuring mode.....                                        | 19        |

|            |                                                                          |           |
|------------|--------------------------------------------------------------------------|-----------|
| <b>7.3</b> | <b>Voltage measurement .....</b>                                         | <b>19</b> |
| 7.3.1      | Automatic measuring mode.....                                            | 19        |
| 7.3.2      | Manual measuring mode .....                                              | 20        |
| <b>7.4</b> | <b>Measuring resistance, capacitance, continuity and diode test.....</b> | <b>20</b> |
| 7.4.1      | testo 770-1/-2 .....                                                     | 20        |
| 7.4.1.1    | Manual measuring mode .....                                              | 20        |
| 7.4.2      | testo 770-3.....                                                         | 21        |
| 7.4.2.1    | Automatic measuring mode .....                                           | 21        |
| 7.4.2.2    | Manual measuring mode .....                                              | 21        |
| <b>7.5</b> | <b>Power measurement (testo 770-3 only) .....</b>                        | <b>21</b> |
| <b>7.6</b> | <b>Frequency measurement .....</b>                                       | <b>22</b> |
| <b>7.7</b> | <b>Temperature measurement (optional) (testo 770-2/-3 only).....</b>     | <b>22</b> |
| 7.7.1      | Carrying out temperature measurement .....                               | 23        |
| <b>7.8</b> | <b>Inrush current (INRUSH) .....</b>                                     | <b>23</b> |
| <b>8</b>   | <b>Service and maintenance .....</b>                                     | <b>24</b> |
| 8.1        | Replacing the batteries .....                                            | 24        |
| 8.2        | Maintenance .....                                                        | 24        |
| 8.3        | Calibration .....                                                        | 25        |
| 8.4        | Storage.....                                                             | 25        |
| 8.5        | Cleaning .....                                                           | 25        |
| <b>9</b>   | <b>Technical data .....</b>                                              | <b>26</b> |
| 9.1        | General technical data .....                                             | 26        |
| 9.2        | More technical data .....                                                | 27        |
| 9.2.1      | testo 770-1/-2 .....                                                     | 27        |
| 9.2.2      | testo 770-3 (0590 7703) .....                                            | 28        |
| 9.2.3      | testo 770-3 (0590 3770 – as of 2024).....                                | 30        |
| 9.3        | Bluetooth module (testo 770-3 only) .....                                | 33        |
| <b>10</b>  | <b>Tips and assistance.....</b>                                          | <b>34</b> |
| 10.1       | Questions and answers.....                                               | 34        |
| 10.2       | Accessories and spare parts.....                                         | 34        |
| <b>11</b>  | <b>Protecting the environment.....</b>                                   | <b>34</b> |

## 2 Observe prior to use!

- The instruction manual contains information and instructions which are necessary for operating and using the instrument safely. Before using the instrument, read the instruction manual carefully and comply with all aspects of it. Keep this document to hand so that you can refer to it when necessary. Forward this documentation to any subsequent users of the instrument.
- If the manual is not followed, or if you fail to observe the warnings and instructions, there is a risk of fatal injury to the user and damage to the instrument.

## 3 Safety instructions

- The instrument may only be used by trained personnel. Please observe the Employers' Liability Insurance Association provisions for health and safety at work.
- Before handling any wires or components, you must first ensure that all power has been shut off to the circuit. It is also recommended to recheck the wires or components for power using a voltage tester.
- According to the description of DIN VDE 0104, this instrument is not approved for **determining the absence of voltage**.
- In order to prevent electrical shock, take safety precautions when working with voltages greater 60 V DC or 30 V AC. Use personal safety equipment such as approved rubber gloves, face protection and flame-resistant clothing.
- Measure a known voltage first to make sure the instrument operates correctly.
- The measuring instrument may only be used with a maximum voltage of 600 V (testo 770-1/-2/-3 (0590 7703)) and 1000 V (testo 770-3 (0590 3770)).
- Measurements that are dangerously close to electrical installations must only be carried out under the direction of a qualified electrician.
- The instrument may only be touched at the designated grip areas, the display elements must not be covered.
- Always ensure that your measuring instrument is in proper working order to maintain operating safety. Decommission the instrument if the following issues apply:
  - has obvious indications of damage
    - cracks on the housing
    - defective test leads
    - leaking batteries
  - will no longer carry out the required measurements
  - was stored for too long in unfavourable conditions
  - was exposed to mechanical stresses during transport.
- Do not use during electrical storms or in wet weather.

- Prevent the instrument from being exposed to extreme heat by direct prolonged sunlight. This is the only way to ensure that the instrument functions perfectly and has a long service life.
- If the instrument needs to be opened, this should only be carried out by an expert. Before being opened, the instrument must be switched off and isolated from all electrical circuits. If you need to open the battery cover, disconnect the test leads before opening the battery cover.
- Maintenance work that is not described in this documentation must only be carried out by trained service technicians.
- If the instrument is modified in any way, operational safety can no longer be guaranteed.
- Modifications or alterations to the instrument will result in warranty or guarantee claims against the manufacturer.
- It is not permitted to use the instrument in an explosive environment.
- Before and after use, always check that the instrument is in peak working order. To do this, test the instrument at a known current source.
- The clamp meter is a portable measuring instrument, suitable for electromagnetic environment for portable equipment or basic electromagnetic environment.

High-frequency electromagnetic fields (HF) can influence the measurement result and result in the wrong information being displayed. This influence is temporary and will not damage the measuring instrument in any way. As soon as the measuring instrument is removed from the influencing HF field, its original accuracy will be re-established. Known sources of these high-frequency electromagnetic fields are radio or mobile telephony equipment, for example. If this type of equipment should influence the measuring instrument, switch it off or increase the distance between the equipment and the measuring instrument.
- The instrument must not be used while its battery compartment is open.
- Batteries must be checked before use and changed if necessary.
- Storage areas must be dry.
- If there is any battery leakage, the instrument must no longer be used until it has been checked by our Customer Service.
- The battery acid (electrolyte) is highly alkaline and electrically conductive. Risk of acid burn! If the battery acid comes into contact with your skin or clothing, thoroughly rinse the areas affected immediately with plenty of water. If battery acid gets into your eyes, rinse them immediately with plenty of water and seek medical advice.

### 4 Intended use

The instrument may only be used under the conditions and for the purpose for which it was designed:

- The instrument conforms to measurement category CAT IV with a rated voltage of 600 V to earth for testo 770-1/-2/-3 (0590 7703), to category CAT IV with a rated voltage of 600 V and CAT III with a rated voltage of 1000 V to earth for testo 770-3 (0590 3770).  
Measurement category CAT IV is for use at the source of voltage installations, e.g. building connection, main fuse, meter. Measurement category CAT III is applicable to test and measuring circuits connected to the distribution part of the building's low-voltage mains installation.

The instrument may only be used in the fields of application described in the instruction manual. Any other application is considered improper and untested usage, and can result in accidents or damage to the instrument. Any misuse will result in the complete invalidation of any warranty or guarantee claims against Testo.

The manufacturer is not responsible for any damage to property or personal injury resulting from the following:

- Failure to observe the instruction manual
- Instrument modifications not approved by the manufacturer
- The use of spare parts not approved by the manufacturer
- Use under the influence of alcohol, drugs or medication

The instrument must not be used for the following circumstances:

- In potentially explosive atmospheres: the instrument is not explosion-proof!
- When there is rain or other precipitation: risk of electric shock!


## 5 Overview

### 5.1 Display and control elements



- 1 Control keys
- 2 LC display
- 3a Clamp trigger (Clamp/hook closed)
- 3b Clamp trigger (Clamp/hook opened)
- 4a Clamp/hook (closed)
- 4b Clamp/hook (opened)
- 5 HOLD key
- 6 Rotary switch
- 7 Grip area
- 8 On the rear: Battery compartment
- 9 Input jack for voltage, resistance, continuity, capacitance, diode, frequency and  $\mu\text{A}$  measurements
- 10. Ground/COM jack for all measurements from point 9

5.2 LC display

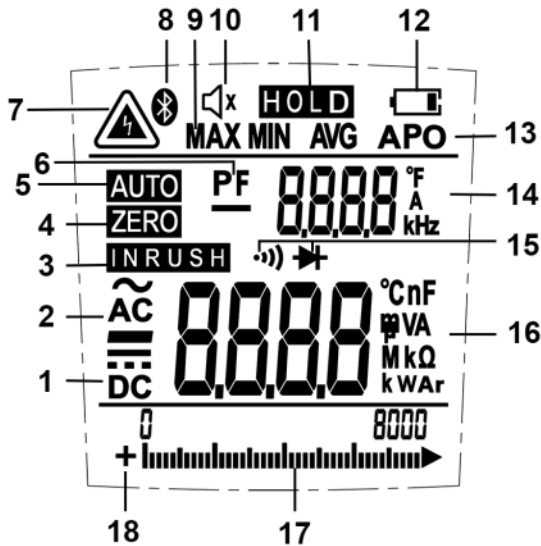

- 1 Direct current/voltage
- 2 Alternating current/voltage
- 3 Inrush current measurement
- 4 Zeroing enabled in DC current measuring mode
- 5 **AUTO** mode
- 6 Power factor
- 7 Dangerous voltage, AC  $\geq 30$  V, DC  $\geq 60$  V
- 8 Bluetooth® enabled (testo 770-3 only)
- 9 Maximum, minimum, average measurement
- 10 Alarm off
- 11 **Hold** is activated, LC display holds the current reading
- 12 Battery capacity display

| Display                                                                                                                    | Feature                                                            |
|----------------------------------------------------------------------------------------------------------------------------|--------------------------------------------------------------------|
| No Symbol                                                                                                                  | Battery capacity 100 – 30 %                                        |
|                                         | Battery capacity 30 – 15 %                                         |
|                                         | Battery capacity 15 – 2 %                                          |
|  flashes and<br>acoustic signal emitted | Battery capacity 2 – 0 %, instrument switches off<br>automatically |

- 13 Automatic power-off function is activated
- 14 Measuring units
- 15 Diode test and continuity
- 16 Measuring units
- 17 Analog display (testo 770-3 only)
- 18 Indication of polarity in bar chart (testo 770-3 only)

### 5.3 Control key functions

The clamp meter features a rotary switch, as well as 6 control keys, which respond to a brief or a long keypress.

In the default setting, the instrument is in **AUTO** mode when voltage, current (testo 770-1/-2/-3 (0590 7703)), RCDC (resistance, capacitance and diode with continuity) is being measured.

| Key                                                                                                                                | Brief keypress <b>function</b> (<1 s)                                                                                                                              | Long keypress <b>function</b> (>2 s)                                                 |
|------------------------------------------------------------------------------------------------------------------------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------------------------------------------------------------------------------------|
| <br>Zero adjustment                               | Zeroing when measuring DC current or DC power                                                                                                                      | Exit zero adjustment                                                                 |
| <br>Select                                        | Switches between the manual sub-modes of the selected measurement.                                                                                                 | Back to <b>AUTO</b> mode                                                             |
| <br>Min/Max                                       | Switches between MAX, MIN and AVG functions                                                                                                                        | Switch off recording mode                                                            |
| <br>Inrush                                        | If position <b>A</b> is selected, the instrument switches to inrush mode.<br><br>Reset the inrush measurement if a measurement is already shown on the LC display. | Switches back to the mode most recently activated before <b>INRUSH</b> was selected. |
| <br>Illumination                                | Background illumination on/off                                                                                                                                     |                                                                                      |
| <br>(testo 770-3)<br>Illumination/<br>Bluetooth | Background illumination on/off                                                                                                                                     | Bluetooth on/off                                                                     |

### 5.4 Rotary switch functions

| Selection                                                                                         | Function                                                                                                                                        |
|---------------------------------------------------------------------------------------------------|-------------------------------------------------------------------------------------------------------------------------------------------------|
| <br>Switch off | Switch the instrument off.                                                                                                                      |
| <br>Current    | Activates automatic mode for current (testo 770-1/-2/-3 (0590 7703)), choose between AC/DC. Manual selection of AC/DC with <b>SELECT</b> .      |
| <br>Voltage    | Activates automatic mode for voltage between AC and DC measurement via the test leads and jacks. Manual selection of AC/DC with <b>SELECT</b> . |

| Selection                                                                                                | Function                                                                                                                                                                                                                                               |
|----------------------------------------------------------------------------------------------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <br>RCDC control        | Automatic mode for resistance, continuity, diode test and capacitance (testo 770-1/-2/-3 (0590 7703)).<br>Automatic mode for resistance and continuity. Manual selection of diode test and capacitance with <b>[SELECT]</b> (testo 770-3 (0590 3770)). |
| <br>testo 770-2/-3 only | Automatic mode for µA measurement. Manual selection of AC/DC with <b>[SELECT]</b> .                                                                                                                                                                    |
| <br>testo 770-3 only    | Activates the mode for power measurement. Manual selection of active, reactive and apparent power, as well as power measurement for direct current/voltage with <b>[SELECT]</b> .                                                                      |

## 5.5 Further functions

### 5.5.1 Bluetooth® (testo 770-3 only)

**testo 770-3 (0590 7703):**

- > Enable Bluetooth®: press and hold down  and turn the rotary switch from **[OFF]** to a function. Then release .
- > Disable Bluetooth®: turn rotary switch to **[OFF]**.

**testo 770-3 (0590 3770):**

- > Enable Bluetooth®: press and hold down  till  appears in the display. Then release .
- > Disable Bluetooth®: press and hold down  till  disappears on the display. Or turn rotary switch to **[OFF]**.

### 5.5.2 HOLD

- > Activate function: press **[HOLD]** <1 s.
- The current reading is recorded and **HOLD** is shown on the LC display.
- > Exit function: press **[HOLD]** <1 s.
- The current measurement is displayed.



The Hold function can be used from all measuring modes.

### 5.5.3 MAX/MIN/AVG

 allows for switching between maximum, minimum and the periodic display of AVG values.

This function is disabled in the default setting.

- > Activate function: press  <1 s.
- Max value is displayed.
- > Display min value and periodic display of AVG values:  
press  <1 s each time.
- > Exit function: press  >2 s or **[HOLD]**.



This function can be activated in all measuring modes (this function is not available at capacitance measurement with testo 770-1 and testo 770-2).



When pressing  in **AUTO AC/DC** voltage mode or **AUTO AC/DC** current measurement mode, the instrument retains the last-selected AC/DC setting. In all other operating states, you can select what you need by briefly pressing the **[SELECT]** key or via the rotary switch itself:

- Voltage measurement (testo 770-1/-2/-3) and measurement with a thermocouple adapter (testo 770-2/-3 (0590 7703) only):  
select .
- Current measurement: select .
- Resistance, continuity, diode and capacitance measurement:  
select .
- $\mu\text{A}$  measurement (testo 770-2, testo 770-3) and measurement with a thermocouple probe or thermocouple adapter (testo 770-3 (0590 3770) only): select .
- Power measurement (testo 770-3 only): select .

## 5.6 Explanation of icons

| Icon                                                                                | Meaning                                                                                                                                                                                                                                                                                                                     |
|-------------------------------------------------------------------------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
|    | <b>Attention!</b> Warning about a danger spot, refer to instruction manual                                                                                                                                                                                                                                                  |
|    | <b>Caution!</b> Dangerous voltage, risk of electric shock                                                                                                                                                                                                                                                                   |
|    | Application around and removal from HAZARDOUS LIVE conductors is permitted.                                                                                                                                                                                                                                                 |
|    | Continuous double or reinforced insulation complies with category II DIN EN 61140 / IEC 536                                                                                                                                                                                                                                 |
|    | The product testo 770-1/-2/-3 (0590 7703) is certified for the US and Canadian markets, in accordance with the applicable American and Canadian standards.                                                                                                                                                                  |
|    | The product testo 770-3 (0590 3770) is certified for the US and Canadian markets, in accordance with the applicable American and Canadian standards.<br>Conforms to UL STD 61010-1, 61010-2-032<br>Certified to CSA STD C22.2 NO. 61010-1, 61010-2-032                                                                      |
|    | Compliance mark for ACMA (Australian Communications and Media Authority) guidelines.                                                                                                                                                                                                                                        |
|   | The product testo 770-1/-2/-3 (0590 7703) has been tested to the requirements of CAN/CSA-C22.2 No. 61010-1, second edition, including Amendment 1, or a later version of the same standard incorporating the same level of testing requirements.                                                                            |
|  | KC (South Korea)                                                                                                                                                                                                                                                                                                            |
|  | Japan certification                                                                                                                                                                                                                                                                                                         |
|  | ANATEL (Brazil)                                                                                                                                                                                                                                                                                                             |
|  | Earth (ground) terminal according to IEC60417                                                                                                                                                                                                                                                                               |
| CAT III                                                                             | Measurement category III is applicable to test and measuring circuits connected to the distribution part of the building's low-voltage mains installation.                                                                                                                                                                  |
| CAT IV                                                                              | Measurement category IV is applicable to test and measuring circuits connected at the source of the building's low-voltage mains installation.                                                                                                                                                                              |
|  | Bluetooth<br>testo 770-3 only                                                                                                                                                                                                                                                                                               |
|  | Conformity mark, verifies compliance with the valid EU Directives: EMC Directive (2014/30/EU) with the EN 61326-1 standard, Low-Voltage Directive (2014/35/EU) with the EN 61010-1 standard.<br>For testo 770-3 (0590 3770): Conformity mark, verifies compliance with the valid EU Directives: RED Directive (2014/53/EU). |
|  | The instrument complies with the WEEE Directive (2012/16/EU)                                                                                                                                                                                                                                                                |

## 6 Operating the instrument

Different measuring modes can be selected via the rotary switch.

When the instrument is in current mode , it automatically detects the range and the type of measurement, AC or DC (testo 770-1/-2/-3 (0590 7703)).

When the instrument is in voltage mode , it automatically detects the range and the type of measurement, AC or DC.

When the rotary switch is at the  position, the instrument measures resistance, continuity, capacitance and diode test.

If the instrument is switched to power mode , it measures active, reactive and apparent power together with the power factor (for sinusoidal signals).



All the available measuring modes can also be selected manually.

### Magnetic suspension system (accessory)



You can use the magnetic suspension system, which is available as an accessory, order number 0590 0001, to attach the testo 770 to metal surfaces.

The suspension system's magnet must not come anywhere near the clamp meter during the measurement (see graphic). Automatic adjustment of the measuring range could be influenced as a result.



Do not hang the testo 770 higher than 2 m.



### WARNING

Magnetic field

May be harmful to those with pacemakers.

> Keep a minimum distance of 15 cm between pacemaker and instrument.

### CAUTION

Magnetic field

Damage to other devices!

> Keep a safe distance away from products that could be damaged by the effects of magnetism (e.g. monitors, computers or credit cards).

### 6.1 Switching the instrument on

- > Switch on: turn the rotary switch to the required measuring mode.
- The instrument switches on.

### 6.2 Switching the background illumination on/off

- > To switch on/off: briefly press the  key.

The background illumination switches off automatically within 2 minutes.



It is possible to switch the background illumination on/off in all measuring modes.

---

### 6.3 Switching the instrument off (automatically/manually)

#### 6.3.1 Automatically

The automatic power-off function (APO) is always enabled as a default setting and is shown on the LC display as **APO**. If no control key is pressed within 15 min, the instrument switches off automatically. If necessary, the automatic power-off function (APO) can be turned off.

- > Disable power-off function: press the  key and turn the rotary switch from the OFF position to a different position.



Once the instrument has switched off, the power-off function is reset to the default setting.

---

#### 6.3.2 Manually

- > Switch off: turn the rotary switch to the **[OFF]** position.

## 6.4 Using testo 770-3 with testo Smart App

### 6.4.1 Establishing Bluetooth® connection (testo 770-3)

You need a tablet or smartphone with the testo Smart App already installed on it to be able to establish a Bluetooth connection.

You can get the App for iOS instruments in the App Store or for Android instruments in the Play Store.

- ✓ The testo Smart App is installed on your mobile terminal device and ready for use.

#### testo 770-3 (0590 7703):

- > Enable Bluetooth®: press and hold down  and turn the rotary switch from **[OFF]** to a function. Then release .
- **CONN** appears in the display. If the Bluetooth® connection is established,  appears in the display and the instrument changes to the set measuring mode.
- > Disable Bluetooth®: Turn rotary switch to **[OFF]**.

#### testo 770-3 (0590 3770):

- > Enable Bluetooth®: press and hold down  until a flashing  appears on the display. Then release .
- If the Bluetooth® connection is established,  stops flashing on the display.
- > Disable Bluetooth®: press and hold down  until  disappears on the display. Or turn rotary switch to **[OFF]**.

### 6.4.2 Transmitting readings

- ✓ testo 770-3 is switched on and connected to your mobile terminal device via Bluetooth.
- The current readings are automatically displayed in the App.

6.4.3 Overview of the App operating controls



|   |                                                                                     |                                                                |
|---|-------------------------------------------------------------------------------------|----------------------------------------------------------------|
| 1 |    | Open main menu                                                 |
| 2 |                                                                                     | Switch between the views (Live, Graphic, Table)                |
| 3 |                                                                                     | Display of the measurement period                              |
| 4 |                                                                                     | Display of connected measuring instruments incl. readings.     |
| 5 |                                                                                     | Buttons <b>[New]</b> , <b>[Start]/[Stop]</b> and <b>[Save]</b> |
| 6 |  | Open Configuration menu                                        |
| 7 |  | Edit reading display                                           |

Further symbols on the user interface (without numbering)

|                                                                                     |                     |
|-------------------------------------------------------------------------------------|---------------------|
|  | One level back      |
|  | Exit view           |
|  | Share report        |
|  | Search              |
|  | Favourite           |
|  | Delete              |
|  | Further information |
|  | Display report      |
|  | Multiple selection  |

## 7 Carrying out a measurement

### 7.1 Preparing for measurement

Prior to every measurement, please ensure that the instrument is in perfect condition:

- For example, keep an eye out for broken housing or leaking batteries.
- Always carry out a function test before using the instrument, see below.
- Check that the instrument is functioning perfectly (for example at a known voltage source) before and after every test.
- If the safety of the user cannot be guaranteed, the instrument must be switched off and secured to prevent unintentional usage.



When connecting the test leads to the test object, always connect the common test lead (**COM**) to the test object first of all. When disconnecting the test leads, always disconnect the +/- phase test lead first of all.

### 7.2 Current measurement



#### WARNING

Serious risk of injury to the user and/or destruction of the instrument while measuring current.

> Measuring circuit must be de-energized.



The measuring instrument may only be used in circuits up to a maximum voltage of 600 V (testo 770-1/-2/-3 (0590 7703)) / 1000 V (testo 770-3 (0590 3770)). The nominal cross-section of the connection cable must be taken into account in order to ensure safe connection (e.g. via crocodile clips).



Strong RF interference and / or open leads when measuring A AC may result in unstable display readings.



For the **A DC** and **µA DC** measurement always zero the instrument with **ZERO** before measuring.

### 7.2.1 Measuring A AC or A DC

#### 7.2.1.1 Automatic measuring mode



For every **DC** current measurement always zero the instrument with  before measuring.

---

1. Switch instrument on: set rotary switch to 
  - The instrument switches on.
  - testo 770-1/-2/-3 (0590 7703): The instrument is in **AUTO A** mode.  
testo 770-3 (0590 3770): The instrument is in manual measuring mode.  
Switch to automatic measuring mode: press  >2 s.
2. Enclose the live conductor and centre it in the jaws.
  - The instrument automatically detects the **A AC** or **A DC** mode.
  - The measured value is shown on the LC display.

#### 7.2.1.2 Manual measuring mode



For every **DC** current measurement always zero the instrument with  before measuring.

---

- ✓ testo 770-1/-2/-3 (0590 7703): Instrument is in automatic measuring mode **AUTO A**
1. Exit **AUTO A** measuring mode: press  <1 s.
  2. Switch between **A AC** and **A DC**: press  <1 s.
- The measured value is shown on the LC display.
- Switch to automatic measuring mode: press  >2 s.
- The instrument is in automatic measuring mode when **AUTO** is illuminated on the LC display.

## 7.2.2 Measuring $\mu\text{A}$ AC or $\mu\text{A}$ DC (testo 770-2/-3 only)

### 7.2.2.1 Automatic measuring mode



For every **DC** current measurement always zero the instrument with  before measuring.

---

1. Switch instrument on: set rotary switch to .
- The instrument switches on.
- The instrument is in **AUTO  $\mu\text{A}$**  mode.
2. Connect test leads: black test lead to black jack, red test lead to red jack. Then connect test leads to the test object.
- The instrument automatically detects the  **$\mu\text{A}$  AC** or  **$\mu\text{A}$  DC** mode.
- The measured value is shown on the LC display.

### 7.2.2.2 Manual measuring mode



For every **DC** current measurement always zero the instrument with  before measuring.

---

- ✓ Instrument is in automatic measuring mode **AUTO  $\mu\text{A}$** .
1. Exit **AUTO  $\mu\text{A}$**  measuring mode: press  <1 s.
  2. Switch between  **$\mu\text{A}$  AC** and  **$\mu\text{A}$  DC**: press  <1 s.
  - The measured value is shown on the LC display.

Switch to automatic measuring mode: press  >2 s.

- The instrument is in automatic measuring mode when **AUTO** is illuminated on the LC display.

## 7.3 Voltage measurement

---



When measuring AC voltage, the frequency is measured at the same time and shown in the relevant row on the LC display.

---

### 7.3.1 Automatic measuring mode

1. Switch instrument on: set rotary switch to .
- The instrument switches on.
- The instrument is in **AUTO V** mode.

## 7 Carrying out a measurement

---

2. Connect test leads: black test lead to black jack, red test lead to red jack.  
Then connect test leads to the test object.
- The measured value is shown on the LC display.

### 7.3.2 Manual measuring mode

- ✓ Instrument is in automatic measuring mode **AUTO V**.
- 1. Exit **AUTO V** measuring mode: press **[SELECT]** <1 s.
- 2. Switch between **V AC** and **V DC**: press **[SELECT]** <1 s.
- The measured value is shown on the LC display.
- 3. Switch to automatic measuring mode: press **[SELECT]** >2 s.
- The instrument is in automatic measuring mode when **AUTO** is illuminated on the LC display.

## 7.4 Measuring resistance, capacitance, continuity and diode test

 **WARNING**

Serious risk of injury to the user and/or destruction of the instrument during resistance testing.

> Test object must be de-energized.



External voltages will distort the measurement result.

### 7.4.1 testo 770-1/-2

#### 7.4.1.1 Manual measuring mode

1. Switch instrument on: set rotary switch to .
- The instrument is switched on.
2. Connect test leads: black test lead to black jack, red test lead to red jack.  
Then connect test leads to the test object.
- The instrument is in **Ω** measuring mode.
3. Switch between resistance, capacitance, continuity and diode test: press **[SELECT]** <1 s.
- The measured value is shown on the LC display.

### 7.4.2 testo 770-3

#### 7.4.2.1 Automatic measuring mode



Automatic detection for resistance and continuity.  
Change to manual measuring mode for diode test and capacitance.

1. Switch instrument on: set rotary switch to .
  - The instrument is switched on.
2. Connect test leads: black test lead to black jack, red test lead to red jack. Then connect test leads to the test object.
  - The instrument is in **AUTO RCDC** measuring mode.
  - The instrument detects resistance and continuity and automatically adjusts the measuring range.
  - The measured value is shown on the LC display.

#### 7.4.2.2 Manual measuring mode

3. Disable **AUTO RCDC** measuring mode: press **[SELECT]** <1 s.
4. Switch between resistance, continuity, diode test and capacitance: press **[SELECT]** <1 s.
  - The measured value is shown on the LC display.
- > Switch back to **AUTO** mode: press **[SELECT]** >2 s.

### 7.5 Power measurement (testo 770-3 only)

For the power measurement, two measurements are carried out at the same time. The voltage of the measurement object is measured via the **COM** jack, **V** input jack and using two test leads. The current of the measurement object must be measured using the clamp meter. From these two factors, the instrument automatically calculates the different types of power, as well as the power factor.



For the **DC** power measurement always zero the instrument with **[ZERO]** before measuring.

1. Switch instrument on: set rotary switch to **W**.
  - The instrument switches on.
  - The instrument is in the mode for power measurement with alternating current/voltage.
2. Enclose the live conductor and centre it in the jaws.

## 7 Carrying out a measurement

---

3. Connect test leads: black test lead to black jack, red test lead to red jack. Then connect test leads to the test object.
4. The instrument displays the active power in w(atts) and the power factor (PF).



The instrument requires approx. 3 s for the reading to be displayed. An updated reading is displayed after approx. 3 s.

---

5. Switch between active power, apparent power, reactive power and power measurement for direct current/voltage: press **SELECT** <1 s.

### 7.6 Frequency measurement

The frequency is displayed automatically during an A AC or V AC measurement.



The following minimum values are necessary for correct display of frequency with voltage and/or current measurement:

Voltage: 1 V

Current: 1.5 % of the measuring range (testo 770-1/-2/-3 (0590 7703))

0.5 % of the measuring range (testo 770-3 (0590 3770))

---

### 7.7 Temperature measurement (optional) (testo 770-2/-3 only)

A thermocouple adapter (0590 0021 for testo 770-2/-3 (0590 7703)) or thermocouple probe (0590 0024 for testo 770-3 (0590 3770)) is optionally available for measuring temperature. Before using the thermocouple adapter or thermocouple probe, please carefully read through the relevant section in the documentation. Familiarize yourself with the product before using it. Pay particular attention to the safety instructions and warning advice in order to prevent injuries and damage to the product.

In this section, it is assumed that you are familiar with the contents of the documentation relating to the thermocouple adapter and thermocouple probe.

### 7.7.1 Carrying out temperature measurement

- ✓ A thermocouple is attached to the thermocouple adapter.
- 1. Switch instrument on: set rotary switch to  (testo 770-2/-3 (0590 7703))  
resp.  (testo 770-3 (0590 3770)).
  - The instrument switches on.
  - The instrument is in **AUTO V / AUTO  $\mu$ A** mode
- 2. Connect the thermocouple (adapter) to the instrument:  
plug the thermocouple (adapter) into the jack. Ensure correct polarity!
  - The thermocouple adapter switches on automatically.
- 3. Activate temperature measurement: press  >2 s.
  - The measured values are shown on the LC display in °C and °F.

### 7.8 Inrush current (INRUSH)



The inrush function is an approximation function. This means that readings can differ from one another.

---

- 1. Switch instrument on: set rotary switch to 
  - The instrument switches on.
  - The instrument is in **AUTO A** mode (testo 770-1/-2/-3 (0590 7703)) resp. **A AC** mode (testo 770-3 (0590 3770)).
- 2. Enclose the live conductor and centre it in the jaws.
- 3. Activate inrush current calculation: press  <1 s.
  - The measured value is shown on the LC display.
- 4. Restart inrush current calculation: press  <1 s.
  - The measured value is shown on the LC display.
- 5. Exit inrush current calculation and switch back to **AUTO A** mode (testo 770-1/-2/-3 (0590 7703)) resp. **A AC** mode (testo 770-3 (0590 3770)):  
press  >2 s.

## 8 Service and maintenance

### 8.1 Replacing the batteries

The batteries need to be replaced when the battery icon appears on the LC display.

- ✓ The instrument is switched off.
- 1. Disconnect the instrument from the test leads and make sure that the instrument is not enclosing any live cable.



- 2. Using a screwdriver, unscrew the two metal screws (1, 2) on the battery compartment until the battery compartment cover can be removed. Do not unscrew the screws completely.
- 3. Remove the spent batteries.
- 4. Insert new batteries, type AAA / IEC LR03 (1.5 V), ensuring correct polarity.
- 5. Put the battery compartment cover back on and screw down.

### 8.2 Maintenance

When operated in accordance with the instruction manual, the instrument does not require any particular maintenance.

If a malfunction occurs during operation, the ongoing measurement should be stopped immediately. Send the instrument to Testo-Industrial-Services GmbH for checking.

### 8.3 Calibration

In order to maintain the specified accuracy of the measurement results, Testo recommends calibrating the instrument once a year. Send the instrument to Testo Service for calibration.

### 8.4 Storage

- Store the instrument in dry, closed rooms.
- > If the instrument is not in use for a significant period of time: remove the batteries in order to prevent any danger or damage due to any potential leaking of the batteries.

### 8.5 Cleaning

Before cleaning, the instrument must be switched off and disconnected from external voltages or from other connected instruments (test specimen, control units, etc.).

- > Wipe the instrument with a damp cloth and a small amount of mild household detergent.

Never use any harsh cleaning agents or solvents to clean the instrument! After being cleaned, the instrument must not be used until it has completely dried.

## 9 Technical data

### 9.1 General technical data

| Feature                                             | Values                                                                                                                                                                      |
|-----------------------------------------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Ambient operating temperature                       | -10 °C to +50 °C                                                                                                                                                            |
| Ambient storage temperature                         | -15 °C to +60 °C                                                                                                                                                            |
| Humidity                                            | 0 to 80 % RH                                                                                                                                                                |
| Operating altitude                                  | Up to 2000 m                                                                                                                                                                |
| Intended use                                        | Indoor use                                                                                                                                                                  |
| Measurement category                                | CAT IV 600 V / CAT III 1000 V                                                                                                                                               |
| Level of contamination                              | 2                                                                                                                                                                           |
| Protection class                                    | IP 40                                                                                                                                                                       |
| Power supply                                        | 3 x 1.5 V (AAA / IEC LR03)                                                                                                                                                  |
| Battery status display                              | Batt. icon appears from <3.9 V                                                                                                                                              |
| Display                                             | 3 3/4 digit, LC display                                                                                                                                                     |
| Display range                                       | testo 770-1/-2: 4000 digits<br>testo 770-3: 6000 digits                                                                                                                     |
| Polarity indicator                                  | automatic                                                                                                                                                                   |
| Overload protection for $\mu$ A current measurement | high-impedance (testo 770-2/-3 only)                                                                                                                                        |
| Inrush current (INRUSH)                             | 100 ms                                                                                                                                                                      |
| Dimensions (H x W x D)                              | 249 x 96 x 44 mm                                                                                                                                                            |
| Weight                                              | 378 g                                                                                                                                                                       |
| Safety standards                                    | WEEE 2012/16/EU, EMC 2014/30/EU, EN 61326-1, Low-Voltage Directive 2014/35/EU with the standard EN 61010-2-032, insulation complies with category II IEC 536 / DIN EN 61140 |

## 9.2 More technical data

### 9.2.1 testo 770-1/-2

| Feature                                                                                            | Measuring range <sup>1</sup>                                        | Resolution                                     | Accuracy                                                                                    |
|----------------------------------------------------------------------------------------------------|---------------------------------------------------------------------|------------------------------------------------|---------------------------------------------------------------------------------------------|
| DC voltage                                                                                         | 4.000 V<br>40.00 V<br>400.0 V<br>600 V                              | 1 mV<br>10 mV<br>100 mV<br>1 V                 | ± (0.8 % of m.v. + 3 digits)                                                                |
| AC voltage <sup>2, 3, 4</sup>                                                                      | 4.000 V<br>40.00 V<br>400.0 V<br>600 V                              | 1 mV<br>10 mV<br>100 mV<br>1 V                 | ± (1.0 % of m.v. + 3 digits)                                                                |
| DC current<br>- jaws [A]<br>- jack [µA]<br>(testo 770-2)                                           | 40 A<br>400 A<br>400 µA                                             | 0.1 A<br>0.1 A<br>0.1 µA                       | ± (2.0 % of m.v. + 5 digit)<br>± (2.0 % of m.v. + 5 digits)<br>± (1.5 % of m.v. + 5 digits) |
| AC current <sup>3</sup><br>- jaws [A] <sup>5</sup><br>- jack [µA]<br>(testo 770-2) <sup>2, 4</sup> | 40 A<br>400 A<br>400 µA                                             | 0.1 A<br>0.1 A<br>0.1 µA                       | ± (2.0 % of m.v. + 5 digit)<br>± (2.0 % of m.v. + 5 digits)<br>± (1.5 % of m.v. + 5 digits) |
| Resistance                                                                                         | 400.0 Ω<br>4.000 kΩ<br>40.00 kΩ<br>400.0 kΩ<br>4.000 MΩ<br>40.00 MΩ | 0.1 Ω<br>1 Ω<br>10 Ω<br>100 Ω<br>1 kΩ<br>10 kΩ | ± (1.5 % of m.v. + 3 digits)                                                                |
| Continuity alarm                                                                                   | <0 ... 30 Ω                                                         |                                                |                                                                                             |
| Diode test                                                                                         | yes (0 to 2.5 V)                                                    |                                                |                                                                                             |
| Capacity                                                                                           | 51.20 nF <sup>6</sup>                                               | 0.01 nF                                        | ± 10 % typically                                                                            |
|                                                                                                    | 512.0 nF                                                            | 0.01 nF                                        | ± (1.5 % of m.v. + 5 digits)                                                                |

<sup>1</sup> The lower measuring ranges are only specified from 5% (does not apply to DC current / AC current measurements with the current probe)

<sup>2</sup> Frequency of AC voltage 40 Hz to 1 kHz

<sup>3</sup> In the case of a mixed signal (AC + DC), only the purely AC component is taken into account

<sup>4</sup> As the frequency increases (over 400 Hz), the accuracy deteriorates  
+/- (2.5% of m.v. + 3 digits) for 400Hz to 750Hz / +/- (5.0% of m.v. + 3digits) for 750Hz to 1000Hz

<sup>5</sup> Frequency of AC current up to 400 Hz

<sup>6</sup> Specification is valid for capacitances > 10 nF

## 9 Technical data

| Feature                                                | Measuring range <sup>1</sup>         | Resolution    | Accuracy                                                                                                        |
|--------------------------------------------------------|--------------------------------------|---------------|-----------------------------------------------------------------------------------------------------------------|
|                                                        | 5.120 $\mu$ F                        | 0.001 $\mu$ F | $\pm$ (1.5% of m.v. + 5 digits)                                                                                 |
|                                                        | 51.20 $\mu$ F                        | 0.01 $\mu$ F  | $\pm$ 10 % typically                                                                                            |
|                                                        | 100.0 $\mu$ F<br>(15 s) <sup>7</sup> | 0.1 $\mu$ F   | $\pm$ 10 % typically                                                                                            |
| Temperature with adapter<br>(testo 770-2) <sup>8</sup> | -20 to 500 °C                        | 0.2 °C        | -20 to 0 °C: $\pm$ 2 °C<br>0 °C to 100 °C: $\pm$ 1 °C<br>100 °C to 250 °C:<br>$\pm$ 1.5 %<br>>250 °C: $\pm$ 2 % |

Figures correspond to +23 °C  $\pm$  5 °C at <80% rel. humidity. Temperature coefficient: 0.15 x specified accuracy per 1 °C (<18 °C and >28 °C)

### 9.2.2 testo 770-3 (0590 7703)

| Feature                                                                                    | Measuring range <sup>9</sup>  | Resolution              | Accuracy                                                             |
|--------------------------------------------------------------------------------------------|-------------------------------|-------------------------|----------------------------------------------------------------------|
| DC voltage                                                                                 | 6.000 V<br>60.00 V<br>600.0 V | 1 mV<br>10 mV<br>100 mV | $\pm$ (0.8 % of m.v. + 3 digits)                                     |
| AC voltage <sup>10, 11, 12</sup>                                                           | 6.000 V<br>60.00 V<br>600.0 V | 1 mV<br>10 mV<br>100 mV | $\pm$ (1.0 % of m.v. + 3 digits)                                     |
| DC current<br>- jaws [A]<br>- jack [ $\mu$ A]                                              | 600 A<br>600 $\mu$ A          | 0.1 A<br>0.1 $\mu$ A    | $\pm$ (2.0 % of m.v. + 5 digits)<br>$\pm$ (1.5 % of m.v. + 5 digits) |
| AC current <sup>11</sup><br>- jaws [A] <sup>13</sup><br>- jack [ $\mu$ A] <sup>10,12</sup> | 600 A<br>600 $\mu$ A          | 0.1 A<br>0.1 $\mu$ A    | $\pm$ (2.0 % of m.v. + 5 digits)<br>$\pm$ (1.5 % of m.v. + 5 digits) |

<sup>7</sup> Maximum measurement duration is 15 s

<sup>8</sup> Does not include the measurement error of the temperature probe. The specified accuracy is the sum total of the measurement errors of the thermocouple adapter and the testo 770.

<sup>9</sup> The lower measuring ranges are only specified from 5% (does not apply to DC current / AC current measurements with the current probe)

<sup>10</sup> Signal bandwidth 40 Hz to 1 kHz

<sup>11</sup> In the case of a mixed signal (AC + DC), only the purely AC component is taken into account

<sup>12</sup> As the frequency increases (over 400 Hz), the accuracy deteriorates  
 $\pm$  (2.5% of m.v. + 3 digits) for 400Hz to 750Hz /  $\pm$  (5.0% of m.v. + 3 digits) for 750Hz to 1000Hz

<sup>13</sup> Frequency of AC currents up to 400 Hz

| Feature                 | Measuring range <sup>9</sup>                                                                                                         | Resolution                                                                                                  | Accuracy                                                                                                                                      |
|-------------------------|--------------------------------------------------------------------------------------------------------------------------------------|-------------------------------------------------------------------------------------------------------------|-----------------------------------------------------------------------------------------------------------------------------------------------|
| Resistance              | 60.00 $\Omega$<br>600.0 $\Omega$<br>6.000 k $\Omega$<br>60.00 k $\Omega$<br>600.0 k $\Omega$<br>6.000 M $\Omega$<br>60.00 M $\Omega$ | 0.01 $\Omega$<br>0.1 $\Omega$<br>1 $\Omega$<br>10 $\Omega$<br>100 $\Omega$<br>1 k $\Omega$<br>10 k $\Omega$ | $\pm (1.5 \% \text{ of m.v.} + 3 \text{ digits})$                                                                                             |
| Continuity alarm        | <0 ... 30 $\Omega$                                                                                                                   |                                                                                                             |                                                                                                                                               |
| Diode test              | yes (0 to 2.5 V)                                                                                                                     |                                                                                                             |                                                                                                                                               |
| Active power            | 600.0 W<br>6.000 kW<br>60.00 kW                                                                                                      | 0.1 W<br>0.001 kW<br>0.01 kW                                                                                | $\pm 5 \% \pm 5 \text{ digit for } I > 10 \text{ A}^{14}$                                                                                     |
|                         | 600.0 kW                                                                                                                             | 0.1 kW                                                                                                      | $\pm 10 \% \pm 5 \text{ digit typical for } 10 \text{ A} > I > 2 \text{ A}^{14}$                                                              |
| Ractive power           | 600.0 VAr                                                                                                                            | 0.1 VAr                                                                                                     | $\pm 5 \% \pm 5 \text{ digit, for } I > 10 \text{ A}^{14}$                                                                                    |
|                         | 6.000 kVAr<br>60.00 kVAr<br>600.0 kVAr                                                                                               | 0.001 kVAr<br>0.01 kVAr<br>0.1 kVAr                                                                         | $\pm 10 \% \pm 5 \text{ digit typical for } 10 \text{ A} > I > 2 \text{ A}^{14}$                                                              |
| Apparent power          | 600.0 VA<br>6.000 kVA<br>60.00 kVA<br>600.0 kVA                                                                                      | 0.1 VA<br>0.001 kVA<br>0.01 kVA<br>0.1 kVA                                                                  | $\pm 1 \text{ digit}^{14}$                                                                                                                    |
| Power for DC/voltage    | 600.0 W<br>6.000 kW<br>60.00 kW<br>600.0 kW                                                                                          | 0.1 W<br>0.001 kW<br>0.01 kW<br>0.1 kW                                                                      | $\pm 1 \text{ digit}^{14}$                                                                                                                    |
| Power factor            | -1.00 to +1.00                                                                                                                       | 0.01                                                                                                        | $\pm 5 \% \pm 5 \text{ digit for } I > 10 \text{ A}^{14}$<br>$\pm 10 \% \pm 5 \text{ digit typical for } 10 \text{ A} > I > 2 \text{ A}^{14}$ |
| Capacitance measurement | 6.000 nF <sup>15</sup>                                                                                                               | 0.001 nF                                                                                                    | $\pm (10 \% \text{ of m.v.} + 25 \text{ digits})$                                                                                             |
|                         | 60.00 nF                                                                                                                             | 0.01 nF                                                                                                     | $\pm (2 \% \text{ of m.v.} + 10 \text{ digits})$                                                                                              |
|                         | 600.0 nF                                                                                                                             | 0.1 nF                                                                                                      | $\pm (1.5 \% \text{ of m.v.} + 5 \text{ digits})$                                                                                             |

<sup>14</sup> Specified measuring accuracy levels for the current and voltage measurement must also be taken into account.

<sup>15</sup> Accuracy valid for capacitance values >2 nF

## 9 Technical data

| Feature                                      | Measuring range <sup>9</sup>      | Resolution                | Accuracy                                                                                                |
|----------------------------------------------|-----------------------------------|---------------------------|---------------------------------------------------------------------------------------------------------|
|                                              | 6.000 $\mu$ F                     | 0.001 $\mu$ F             | $\pm$ (1.5 % of m.v. + 5 digits)                                                                        |
|                                              | 60.00 $\mu$ F                     | 0.01 $\mu$ F              | $\pm$ (1.5 % of m.v. + 5 digits)                                                                        |
|                                              | 600.0 $\mu$ F                     | 0.1 $\mu$ F               | $\pm$ (2 % of m.v. + 10 digits)                                                                         |
|                                              | 6.000 mF                          | 1 $\mu$ F                 | $\pm$ 10 % typically                                                                                    |
|                                              | 60.00 mF <sup>16</sup>            | 10 $\mu$ F                | $\pm$ 10 % typically                                                                                    |
| Frequency with voltage/current <sup>17</sup> | 99.99 Hz<br>999.9 Hz<br>9.999 kHz | 0.01 Hz<br>0.1 Hz<br>1 Hz | $\pm$ (0.1 % + 1 digits)                                                                                |
| Temperature with adapter <sup>18</sup>       | -20 to 500 °C                     | 0.2 °C                    | -20 to 0 °C $\pm$ 2 °C<br>0 to 99.99 °C $\pm$ 1 °C<br>100 to 249.99 °C $\pm$ 1.5 %<br>>250 °C $\pm$ 2 % |

Figures correspond to +23 °C  $\pm$  5 °C at <80 % rel. humidity. Temperature coefficient: 0.15 x specified accuracy per 1 °C (<18 °C and >28 °C)

### 9.2.3 testo 770-3 (0590 3770 – as of 2024)

| Feature                      | Measuring range <sup>19</sup> | Resolution | Accuracy                         |
|------------------------------|-------------------------------|------------|----------------------------------|
| DC voltage                   | 600.0 mV                      | 0.1 mV     | $\pm$ (0.5 % of m.v. + 4 digits) |
|                              | 6.000 V                       | 0.001 V    |                                  |
|                              | 60.00 V                       | 0.01 V     |                                  |
|                              | 600.0 V                       | 0.1 V      | $\pm$ (0.8 % of m.v. + 5 digits) |
|                              | 1000.0 V                      | 1 V        |                                  |
| AC voltage <sup>20, 21</sup> | 6.000 V                       | 0.001 V    | $\pm$ (0.9 % of m.v. + 5 digits) |
|                              | 60.00 V                       | 0.01 V     |                                  |
|                              | 600.0 V                       | 0.1 V      |                                  |
|                              | 1000 V                        | 1 V        | $\pm$ (1.2 % of m.v. + 5 digits) |

<sup>16</sup> Maximum measurement duration is 13.2 s

<sup>17</sup> Frequency measurement is not specified for alternating currents or voltages below 3% of the smallest respective measuring range

<sup>18</sup> Does not include the measurement error of the temperature probe. The specified accuracy is the sum total of the measurement errors of the thermocouple adapter and the testo 770

<sup>19</sup> The lower measuring ranges are only specified from 5% (does not apply to DC current / AC current measurements with the current probe)

<sup>20</sup> Signal bandwidth 45 Hz to 1 kHz

<sup>21</sup> In the case of a mixed signal (AC + DC), only the purely AC component is taken into account

| Feature                       | Measuring range <sup>19</sup>                                                  | Resolution                                                              | Accuracy                                                                                                                                        |
|-------------------------------|--------------------------------------------------------------------------------|-------------------------------------------------------------------------|-------------------------------------------------------------------------------------------------------------------------------------------------|
| DC current                    |                                                                                |                                                                         |                                                                                                                                                 |
| - jaws [A]                    | 60.00 A<br>600.0 A                                                             | 0.01 A<br>0.1 A                                                         | ± (2.0 % of m.v. + 5 digits)                                                                                                                    |
| - jack [μA]                   | 600.0 μA                                                                       | 0.1 μA                                                                  | ± (1.5 % of m.v. + 5 digits)                                                                                                                    |
| AC current                    |                                                                                |                                                                         |                                                                                                                                                 |
| - jaws [A] <sup>22, 23</sup>  | 3.00 A<br>60.00 A<br>600.0 A                                                   | 0.01 A<br>0.01 A<br>0.1 A                                               | ± (2.0 % of m.v. + 15 digits)<br>± (2.0 % of m.v. + 5 digits)                                                                                   |
| - jack [μA] <sup>20, 22</sup> | 600.0 μA                                                                       | 0.1 μA                                                                  | ± (1.5 % of m.v. + 5 digits)                                                                                                                    |
| Resistance                    | 60.00 Ω<br>600.0 Ω<br>6.000 kΩ<br>60.00 kΩ<br>600.0 kΩ<br>6.000 MΩ<br>60.00 MΩ | 0.01 Ω<br>0.1 Ω<br>0.001 kΩ<br>0.01 kΩ<br>0.1 kΩ<br>0.001 MΩ<br>0.01 MΩ | ± (1.2 % of m.v. + 5 digits)<br>± (1.2 % of m.v. + 3 digits)<br><br><br><br>± (1.5 % of m.v. + 3 digits)<br>± (2.5 % of m.v. + 5 digits)        |
| Continuity alarm              | 0 to 30 Ω                                                                      |                                                                         |                                                                                                                                                 |
| Diode test                    | yes (0 to 3 V)                                                                 |                                                                         |                                                                                                                                                 |
| Active power                  | 600.0 W<br>6.000 kW<br>60.00 kW                                                | 0.1 W<br>0.001 kW<br>0.01 kW                                            | ± (15 % of m.v. + 15 digits)<br>for I = 1 to 10 A, V > 10 V <sup>24</sup><br>± (5 % of m.v. + 5 digits)<br>for I > 10 A, V > 10 V <sup>24</sup> |
|                               | 600.0 kW                                                                       | 0.1 kW                                                                  | ± (10 % of m.v. + 5 digits)<br>for I > 10 A, V > 10 V <sup>24</sup>                                                                             |
| Reactive power                | 600.0 VAr                                                                      | 0.1 VAr                                                                 | ± (15 % of m.v. + 15 digits)<br>for I = 1 A to 10 A, V > 10 V<br>± (5 % of m.v. + 5 digits)<br>for I > 10 A, V > 10 V <sup>24</sup>             |
|                               | 6.000 kVAr<br>60.00 kVAr<br>600.0 kVAr                                         | 0.001 kVAr<br>0.01 kVAr<br>0.1 kVAr                                     | ± (10 % of m.v. + 5 digits)<br>for I > 10 A, V > 10 V <sup>24</sup>                                                                             |

<sup>22</sup> Frequency of AC currents 45 Hz to 400 Hz. Do not exceed the rated frequency, which will cause the magnetic circuit temperature to be too high, resulting in thermal hazards.

<sup>23</sup> Accuracy valid for current values > 0.3 A

<sup>24</sup> Specified measuring accuracy levels for the current and voltage measurement must also be taken into account.

## 9 Technical data

| Feature                              | Measuring range <sup>19</sup>                   | Resolution                                 | Accuracy                                                                                                                              |
|--------------------------------------|-------------------------------------------------|--------------------------------------------|---------------------------------------------------------------------------------------------------------------------------------------|
| Apparent power                       | 600.0 VA<br>6.000 kVA<br>60.00 kVA<br>600.0 kVA | 0.1 VA<br>0.001 kVA<br>0.01 kVA<br>0.1 kVA | ± (15 % of m.v. + 15 digits)<br>for I = 1 A to 10 A, V > 10 V<br>± (2.0 % of m.v. + 5 digits)<br>for I > 10 A, V > 10 V <sup>14</sup> |
| Power for DC/voltage                 | 600.0 W<br>6.000 kW<br>60.00 kW<br>600.0 kW     | 0.1 W<br>0.001 kW<br>0.01 kW<br>0.1 kW     | ± (15 % of m.v. + 15 digits)<br>for I = 1 A to 10 A, V > 10 V<br>± (2.0 % of m.v. + 5 digits)<br>for I > 10 A, V > 10 V <sup>24</sup> |
| Power factor                         | -1.00 to +1.00                                  | 0.01                                       | ± (5 % of m.v. + 5 digits)<br>for I > 10 A, V > 10 V <sup>24</sup>                                                                    |
| Capacitance measurement              | 6.000 nF <sup>25</sup>                          | 0.001 nF                                   | ± (10 % of m.v. + 25 digits)                                                                                                          |
|                                      | 60.00 nF                                        | 0.01 nF                                    | ± (2 % of m.v. + 25 digits)                                                                                                           |
|                                      | 600.0 nF                                        | 0.1 nF                                     | ± (1.5 % of m.v. + 5 digits)                                                                                                          |
|                                      | 6.000 µF                                        | 0.001 µF                                   | ± (1.5 % of m.v. + 5 digits)                                                                                                          |
|                                      | 60.00 µF                                        | 0.01 µF                                    | ± (1.5 % of m.v. + 5 digits)                                                                                                          |
|                                      | 600.0 µF                                        | 0.1 µF                                     | ± (2 % of m.v. + 10 digits)                                                                                                           |
|                                      | 6.000 mF                                        | 1 µF                                       | ± 10 % of m.v.                                                                                                                        |
|                                      | 60.00 mF <sup>26</sup>                          | 10 µF                                      | ± 10 % of m.v.                                                                                                                        |
| Frequency with voltage <sup>27</sup> | 99.99 Hz<br>999.9 Hz<br>9.999 kHz               | 0.01 Hz<br>0.1 Hz<br>0.001 kHz             | ± (0.08 % of m.v. + 3 digits)                                                                                                         |
| Frequency with current <sup>17</sup> | 99.99 Hz<br>999.9 Hz<br>9.999 kHz               | 0.01 Hz<br>0.1 Hz<br>0.001 kHz             | ± (0.08 % of m.v. + 3 digits)<br>for I > 2 A<br>± (0.1 % of m.v. + 15 digits)<br>for 0.6 A < I < 2 A <sup>28</sup>                    |

<sup>25</sup> Accuracy valid for capacitance values >2 nF

<sup>26</sup> Maximum measurement duration is 12.2 s

<sup>27</sup> Frequency measurement is not specified for alternating currents or voltages below 1 % of the smallest respective measuring range

<sup>28</sup> 40~1kHz

| Feature                                         | Measuring range <sup>19</sup> | Resolution | Accuracy                                                                                                                               |
|-------------------------------------------------|-------------------------------|------------|----------------------------------------------------------------------------------------------------------------------------------------|
| Temperature with probe or adapter <sup>29</sup> | -20 to 500 °C                 | 0.2 °C     | -20 to 0 °C ± 2 °C<br>0 to 99.99 °C ± (0.7 % of m.v. + 1.2 °C)<br>100 to 249.99 °C ± (1.4 % of m.v. + 0.5 °C)<br>>250 °C ± 2 % of m.v. |

Figures correspond to +23 °C ± 5 °C at <80 % rel. humidity. Temperature coefficient: 0.15 x specified accuracy per 1 °C (< 18 °C and > 28 °C)

### 9.3 Bluetooth module (testo 770-3 only)



The use of the wireless module is subject to the regulations and stipulations of the respective country of use, and the module may only be used in each case in countries for which a country certification has been granted.

The user and every owner undertake to adhere to these regulations and prerequisites for use, and acknowledge that the re-sale, export, import, etc. in particular in, to or from countries without wireless permits, is their responsibility.

<sup>29</sup> Does not include the measurement error of the temperature probe. The specified accuracy is the sum total of the measurement errors of the thermocouple probe or thermocouple adapter and the testo 770-3.

## 10 Tips and assistance

### 10.1 Questions and answers

| Question                          | Possible causes/solution                                                                                                                      |
|-----------------------------------|-----------------------------------------------------------------------------------------------------------------------------------------------|
| <b>OL</b>                         | The reading exceeds the measuring range upper limit<br>> Check input value and change if necessary.                                           |
| <b>dISC</b><br>(testo 770-3 only) | The capacitor to be tested still contains charge.<br>> Discharge capacitor properly and carry out the test again.                             |
| <b>OPEn</b>                       | No connection to the probe tips during the RCDC measuring mode.<br>> Establish a connection to the measurement object.                        |
| <b>UPdE bLE</b>                   | Update Bluetooth<br>> Wait up to 30s.<br>> If no connection is established reset Bluetooth connection, restart testo Smart App and try again. |

If we have not been able to answer your question, please contact your dealer

### 10.2 Accessories and spare parts

Probe and other assemblies are appropriately rated for measurement category III or IV and have a suitable voltage rating for the circuit to be measured.

## 11 Protecting the environment

- > Dispose of faulty rechargeable batteries/spent batteries in accordance with the valid legal specifications.
- > At the end of its useful life, send the product to the separate collection for electric and electronic devices (observe local regulations) or return the product to Testo for disposal.