

User manual

Temperature Calibrator

JOFRA ITC-155/320/650 A

© Copyright 2001 AMETEK DENMARK A/S



FIG. 1

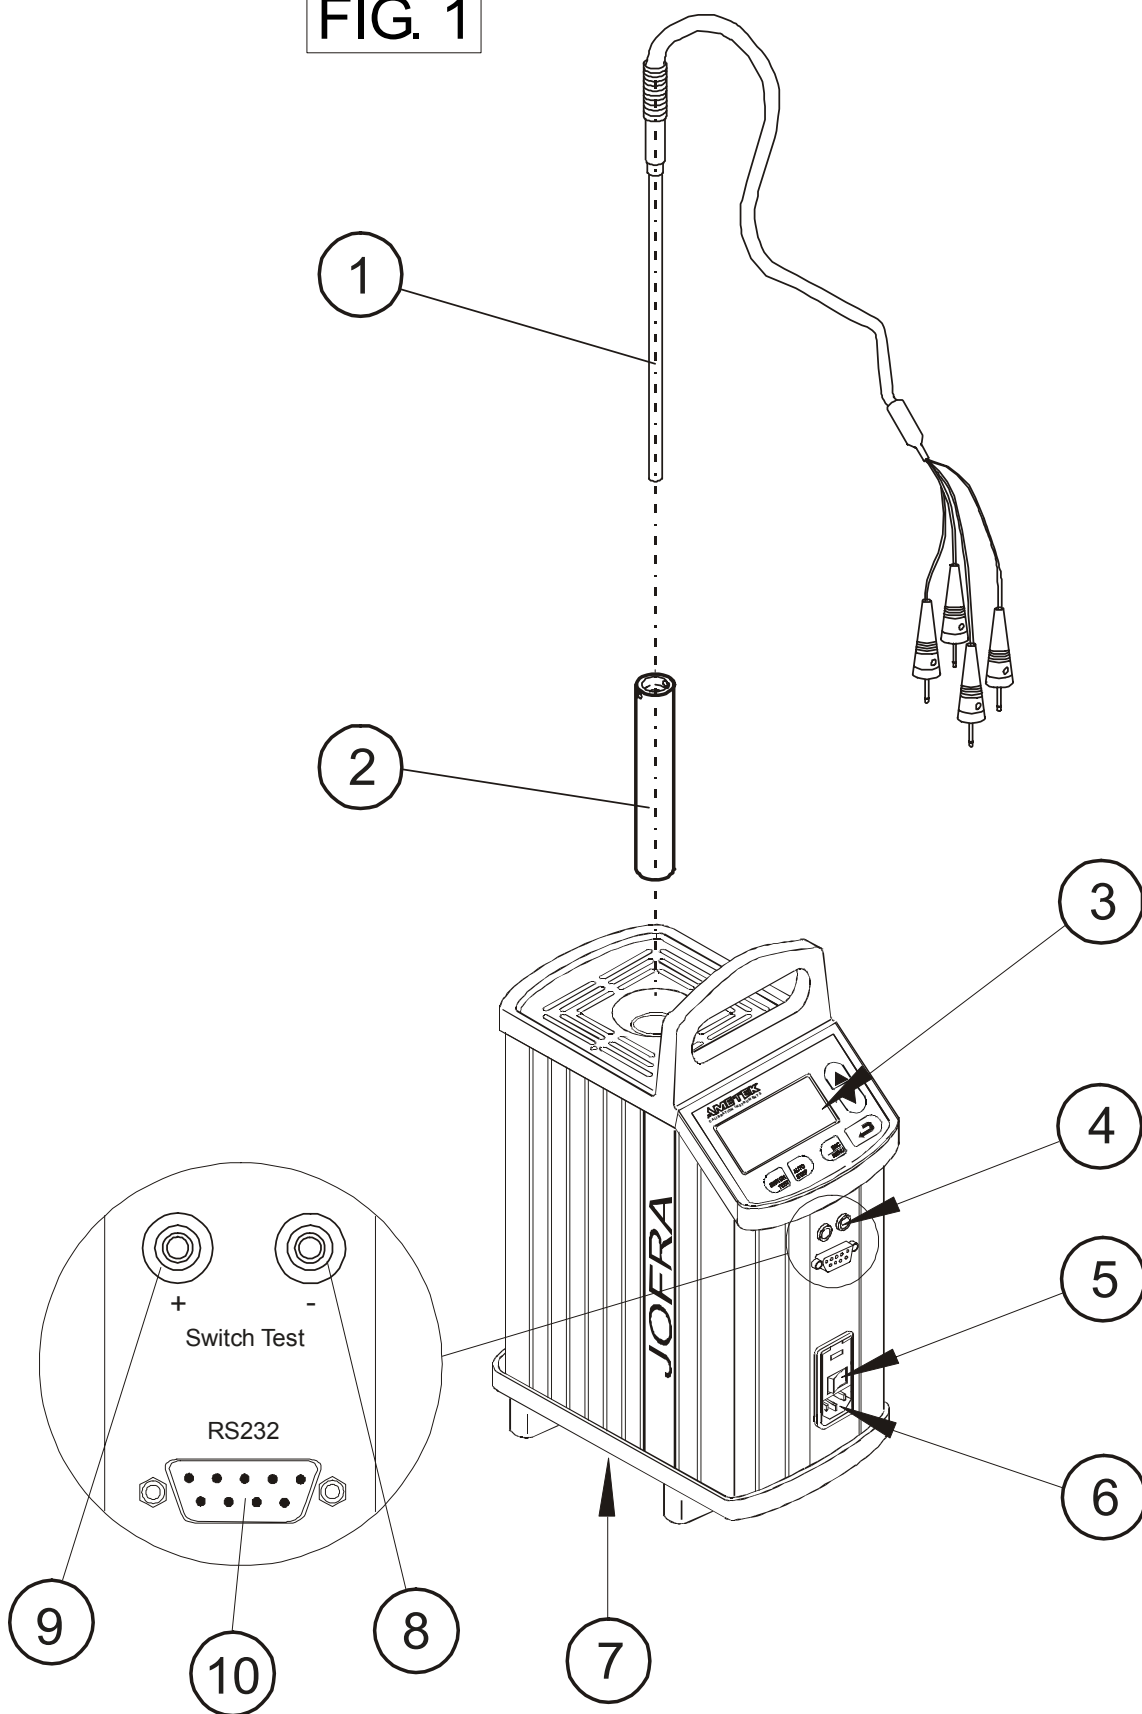


FIG. 2

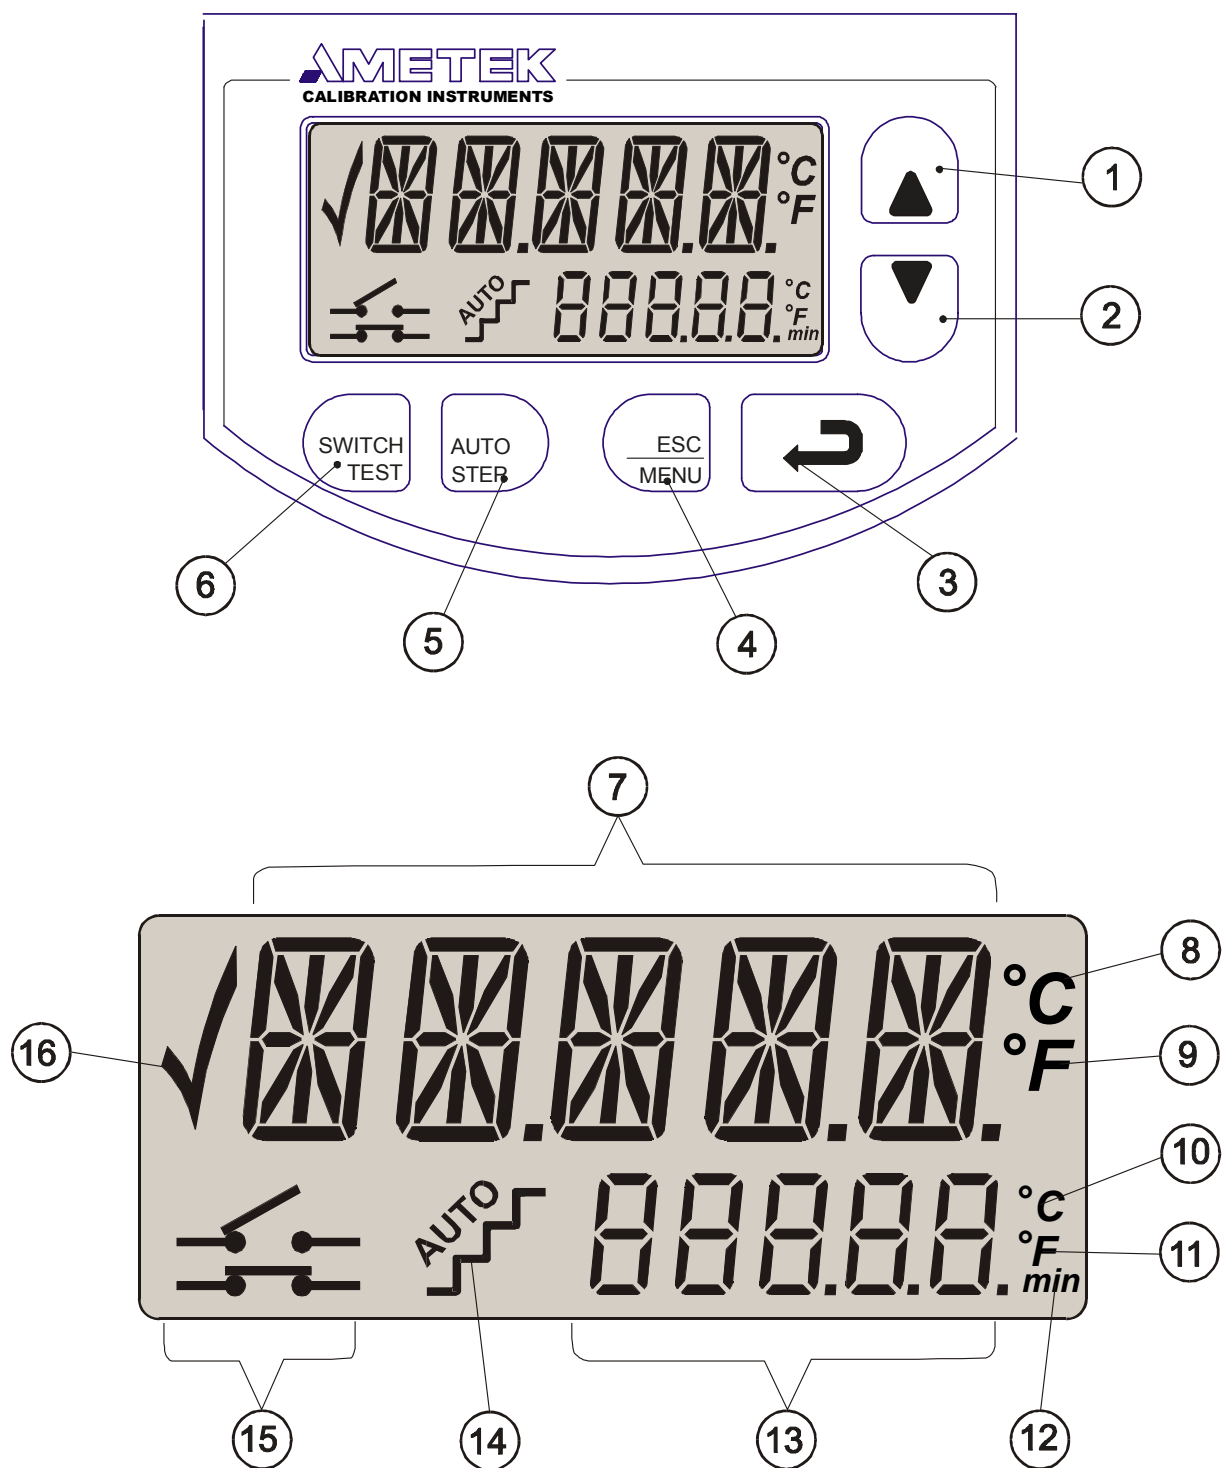


FIG. 3

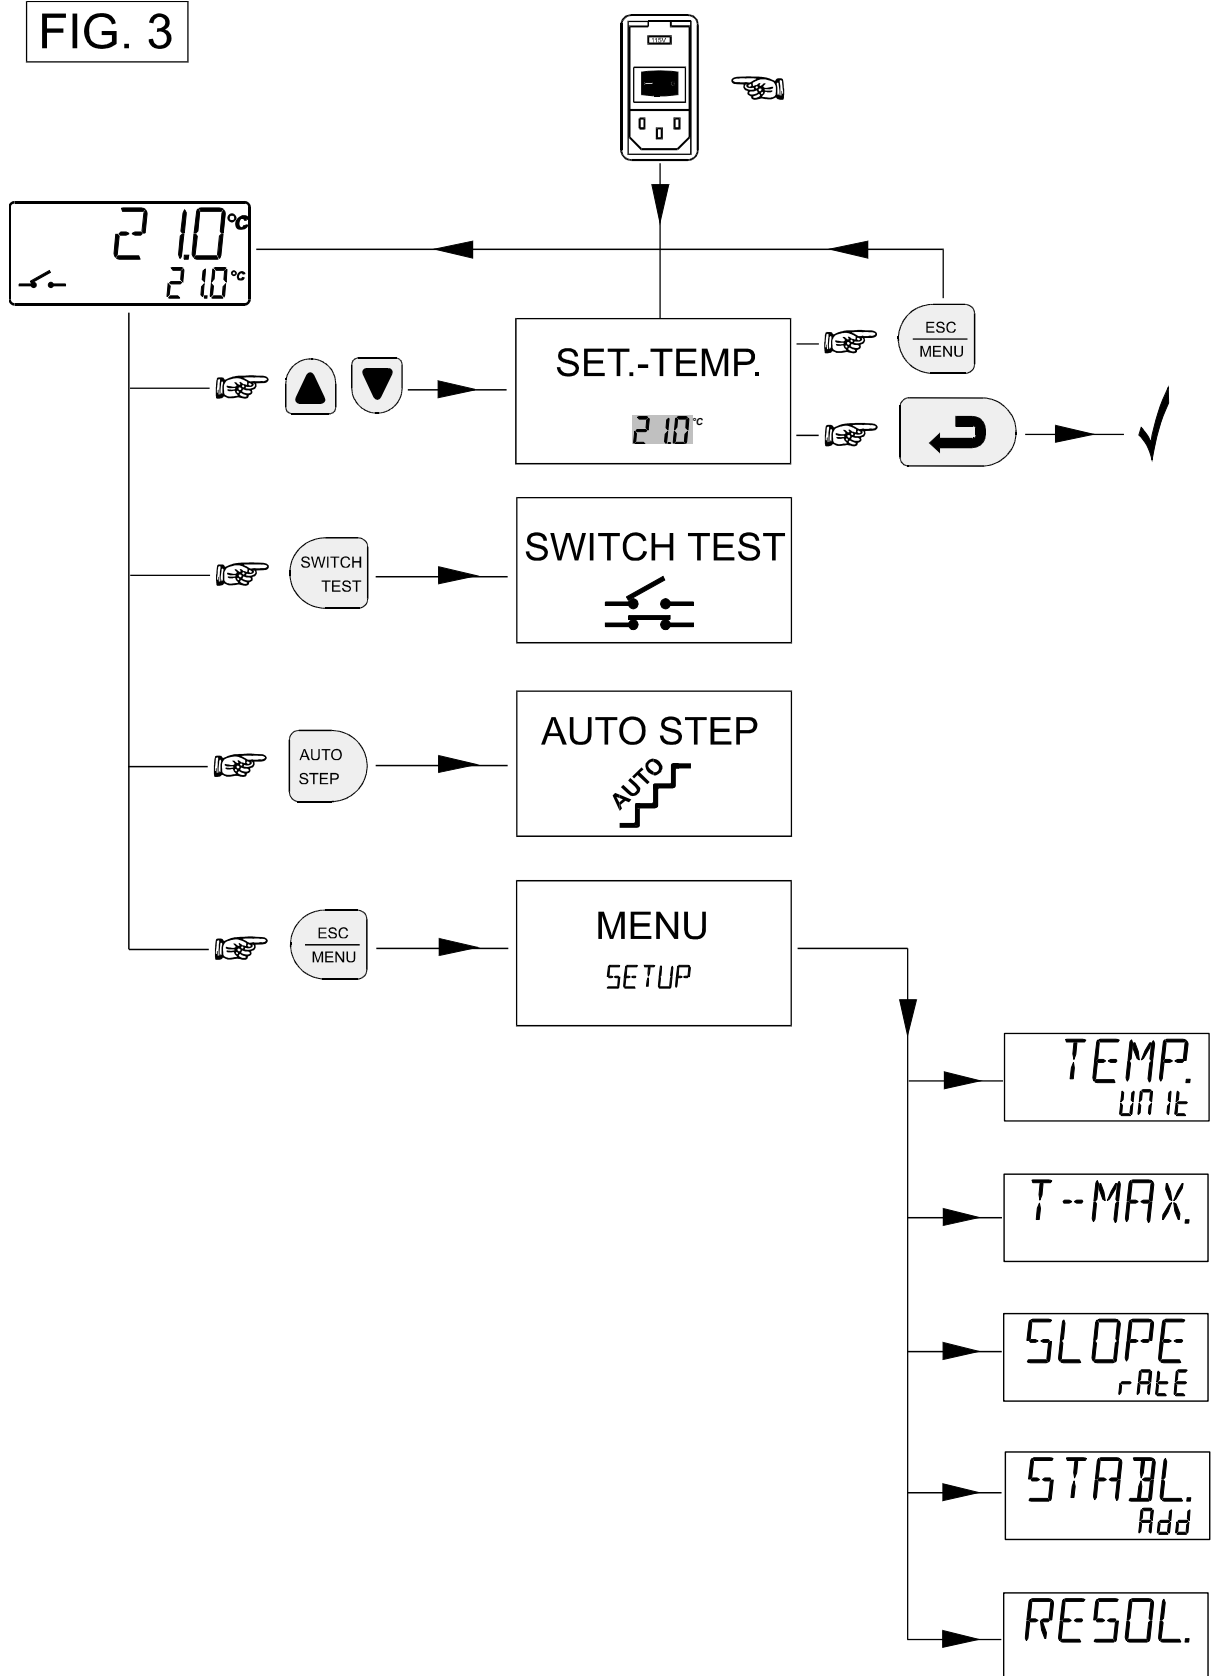


FIG. 4

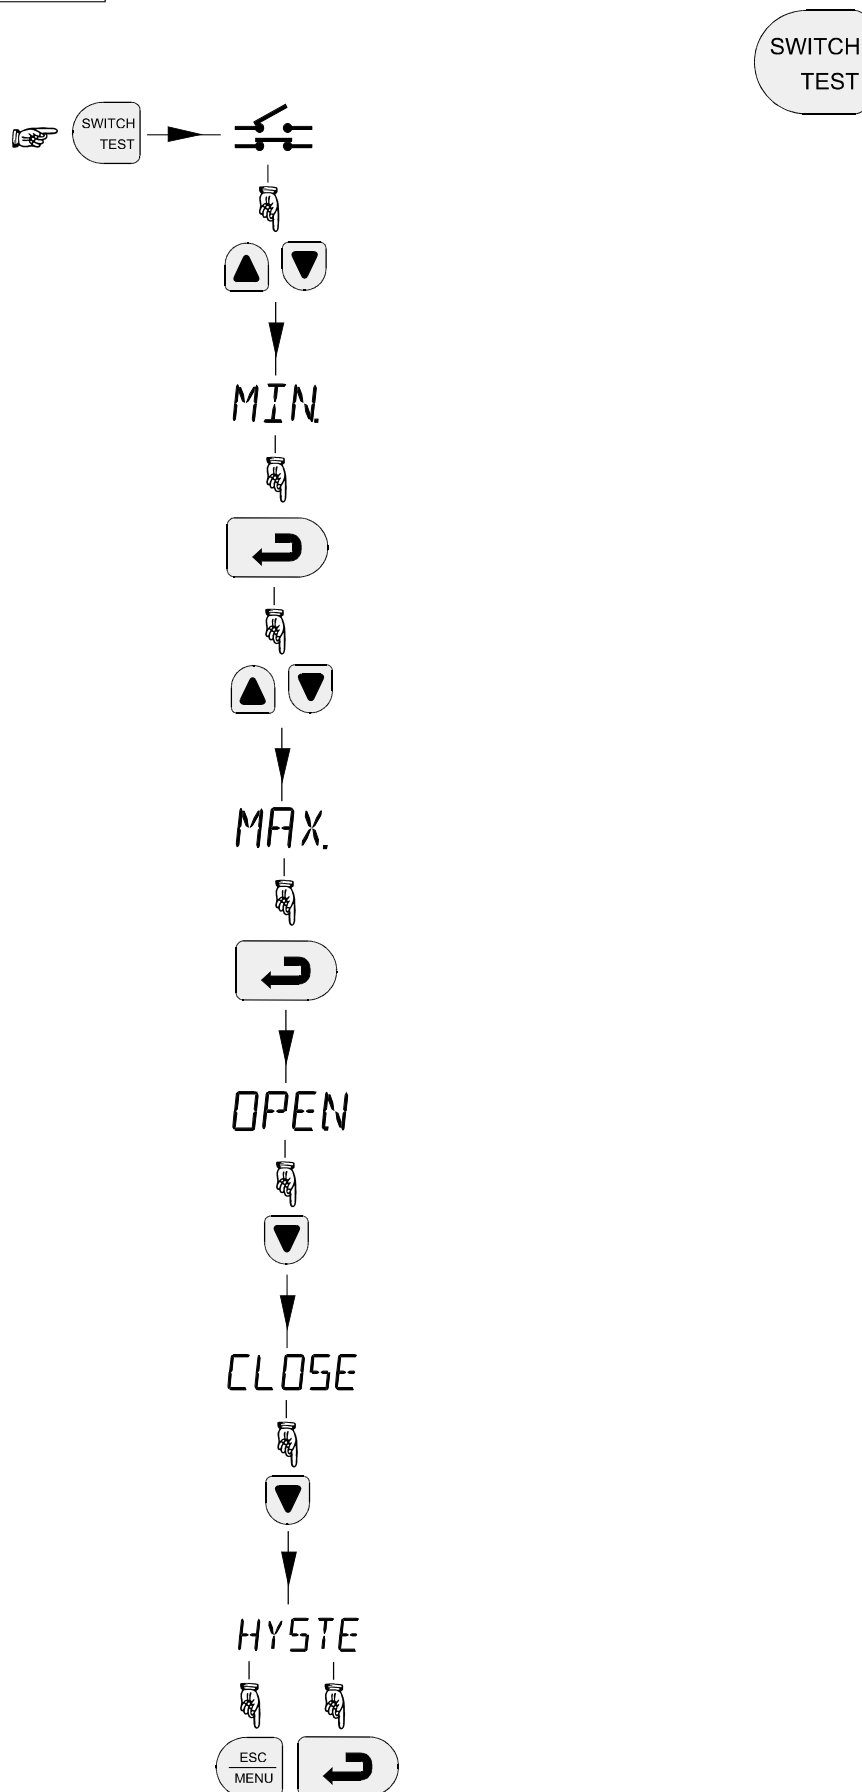


FIG. 5


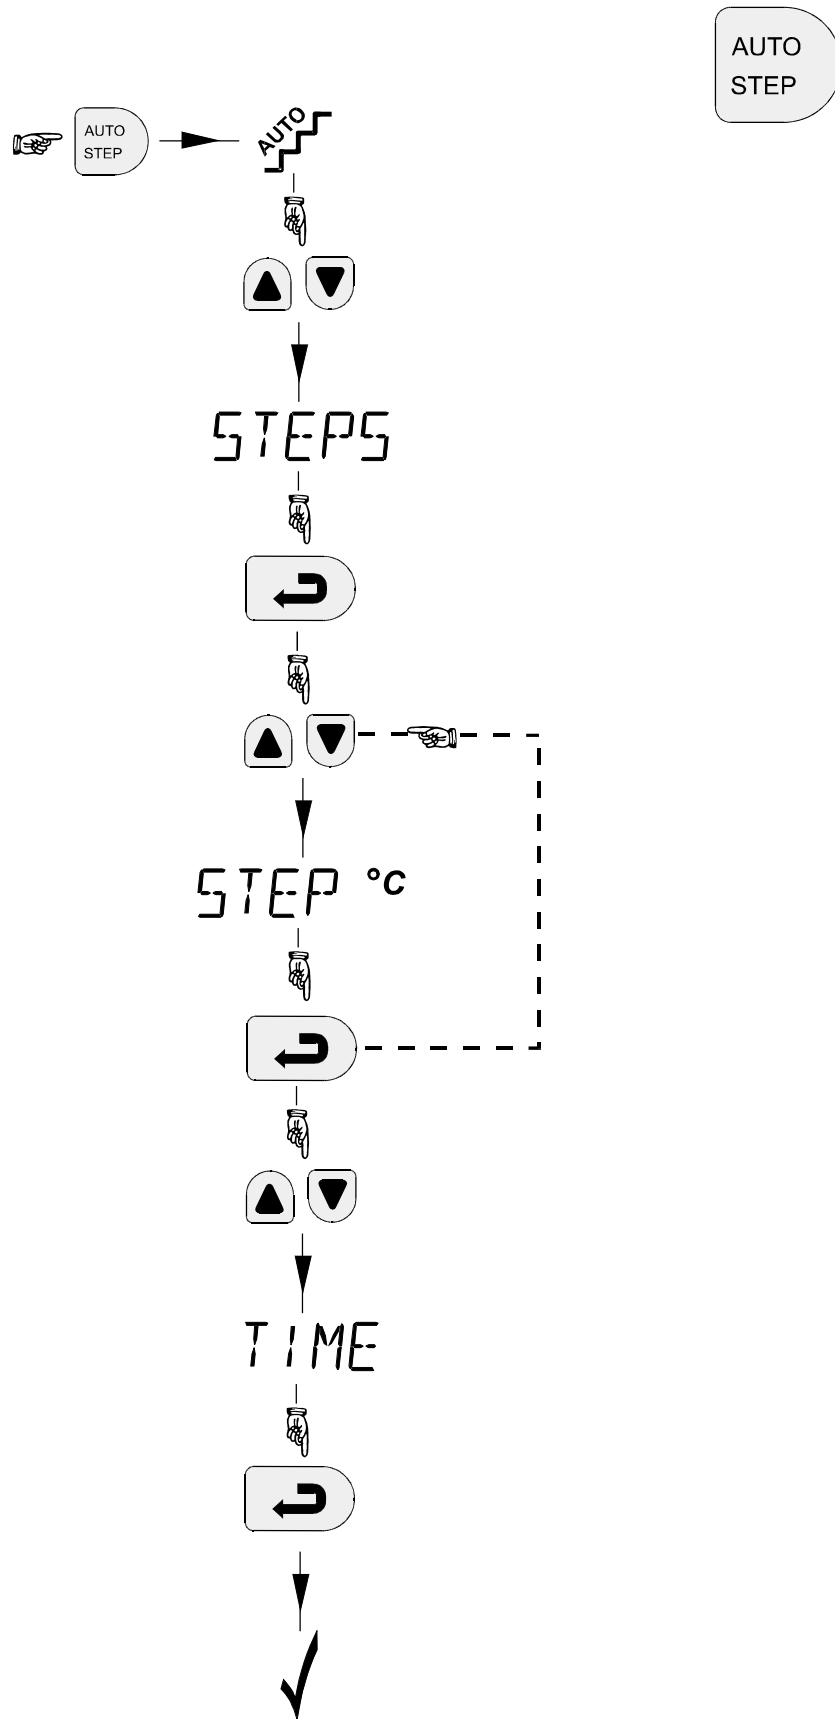


FIG. 6

ESC
MENU

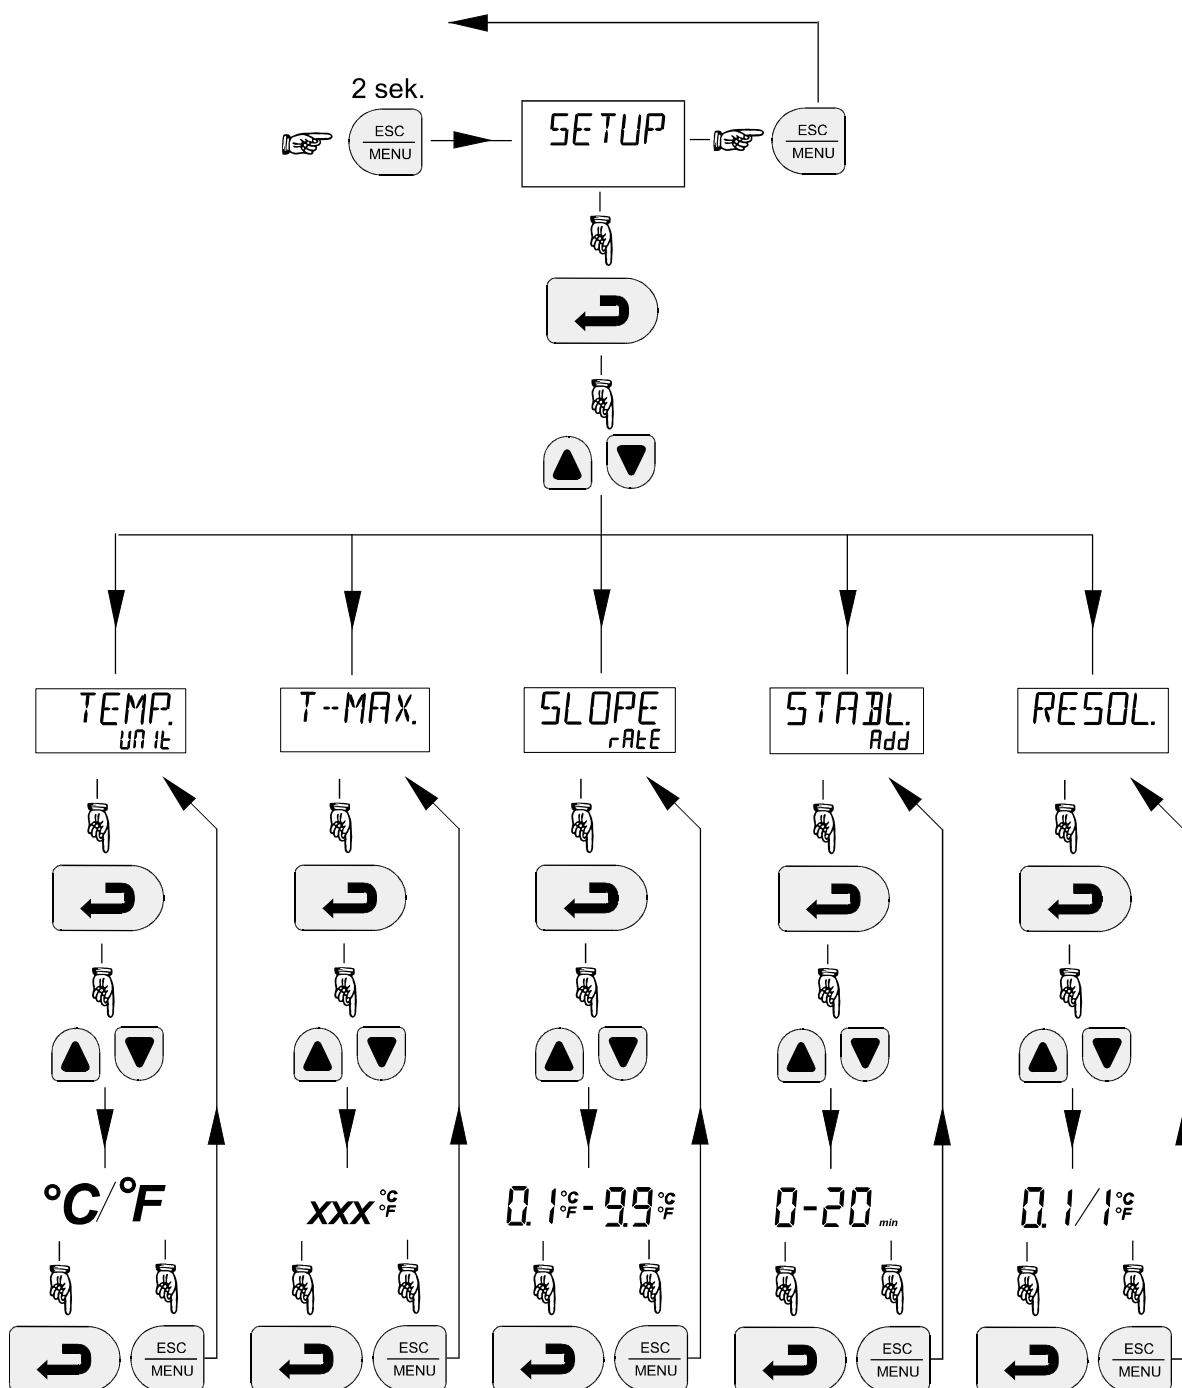

.....ENGLISH

List of contents

1.0	Introduction	2
1.1	List of equipment received	2
2.0	Operating the calibrator	3
2.1	Before use	3
2.2	Keyboard	5
2.3	Display	5
2.4	Connections	6
2.5	Calibrator functions - overview	6
2.6	Selecting the set-temperature	6
2.7	SWITCH TEST	7
2.8	AUTO STEP	8
2.9	MENU	9
3.0	Setting the main voltage and replacing the fuses.....	10
4.0	After use	12

1.0 Introduction

ITC-calibrators are temperature calibrators designed to calibrate temperature sensors and temperature switches.

Read this manual carefully before using the instrument and make sure that all safety instructions and warnings are observed.

1.1 List of equipment received

When you receive the instrument, the following should be enclosed:

- 1 calibrator
- 1 mains cable
- 1 set of test cables (1 black, 1 red)
- 1 insertion tube for 6 mm sensors
- 1 tool for insertion tube
- 1 traceable certificate
- 1 reference manual
- 1 user manual
- RS232 serial cable
- 1 CD-ROM containing software package “AmeCal Temperature”
(The adjustment software “AmeTrim” is **not** applicable to the ITC-calibrators)

2.0 Operating the calibrator

2.1 Before use



Warning

- The calibrator **must not** be used for any purposes other than those described in this manual.
- The calibrator is designed for **interior use only** and should **not be used in risk-prone areas**, where vapour or gas leaks, etc. may constitute an explosives hazard.
- The connections used to test thermostats (Fig. 1 pos. 8 and 9) must **NEVER** be connected to voltages exceeding 50V. The thermostats must not be connected to any other source of voltage during the test.
- **NEVER** use heat transfer fluids such as silicone, oil, paste, etc.
- The calibrator **must** be kept clear within an area of 20 cm on all sides and 1 metre above the calibrator.



Caution – Hot surface

This symbol is engraved in the grid plate.

- **Do not touch** the grid plate, the well or the insertion tube as the calibrator is heating up – they may be very hot.
- **Do not touch** the handle of the calibrator during use – it may be very hot.

Follow the instructions below before using the calibrator (cf. Fig. 1):

1. Place the calibrator on an even horizontal surface away from all draughts.



Caution...

Do not use the instrument if the ventilator is out of order. Ensure a free supply of air to the ventilator located at the bottom of the instrument (pos. 7).

2. Check that the voltage shown on the power control switch (pos. 5) is identical to the mains voltage.
3. Plug in the cable below the power control switch (pos. 6) and check that the earth connection is present.
4. Select an insertion tube (pos. 2) with a well diameter that matches the sensor (pos. 1) to be calibrated. Insert the insertion tube in the well of the calibrator (note that the well and the insertion tube **must** be clean before use).
5. Place the sensor (pos. 1) in the insertion tube (pos. 2) as shown in Fig. 1.
6. In order to spare the sensor and its connections it is recommended to use a heat protection shield (104216) at high temperatures.

2.2 Keyboard

The keys on the keyboard activate the following functions (cf. Fig. 2):

POS	Description
①	UP ARROW button used to adjust temperature values (value increases) and to select menu options.
②	DOWN ARROW button used to adjust temperature values (value decreases) and to select menu options.
③	ENTER button used to accept chosen options.
④	ESC/MENU button used to escape or to activate the menu system (hold button down for min. 2 seconds).
⑤	AUTO STEP button used to activate AUTO STEP. The function is used to switch between a series of set-temperatures automatically.
⑥	SWITCH TEST button used to activate SWITCH TEST. The function automatically detects the opening/closing temperatures for thermostats.

2.3 Display

The various segments of the display are used to indicate the following (cf. Fig. 2):

POS	Description
⑦	Used to display Read-temperature and parameters in the menu system.
⑧	Celsius temperature unit for top display.
⑨	Fahrenheit temperature unit for top display.
⑩	Celsius temperature unit for bottom display.
⑪	Fahrenheit temperature unit for bottom display.
⑫	Minute time unit for bottom display.

- ⑬ Used to display set-temperature, time-until-stable and parameter values in the menu system.
- ⑭ AUTO STEP symbol used to indicate that the function is active (symbol flashes repeatedly).
- ⑮ SWITCH TEST input closed.
SWITCH TEST input open.
- ⑯ Check mark displayed when the calibrator is stable.

2.4 Connections


The instrument is designed for the following connections (cf. Fig. 1):

POS	Description
⑧	Connection of black test cable -
⑨	Connection of red test cable +
⑩	Connection of RS232 cable
	Note that all PC-equipment, which are connected to the calibrator must observe the directive IEC950.

2.5 Calibrator functions - overview

The instrument's functions are divided into hierarchical groups. See the key diagram in Fig. 3.

2.6 Selecting the set-temperature

-  Press  or . The current set-temperature flashes (the starting point is the last chosen set-temperature even if the instrument has been switched off).
-  Press  or  to select the required temperature.
-  Press  to accept the change or  to cancel and return to the previous value.


The calibrator will now work towards the new set-temperature.

2.7 SWITCH TEST

The SWITCH TEST function (cf. Fig. 4) automatically locates the opening/closing temperatures of a thermostat. You must enter a $T_{\min}$ - and a $T_{\max}$ -temperature which define the range within which the opening/closing temperatures are expected to be found.

 Press . The last chosen $T_{\min}$ -temperature value will flash.

 Press  or  to set the required $T_{\min}$ -temperature.

 Press  to accept your selection.

 Press  or  to set the required $T_{\max}$ -temperature.

 Press  to accept your selection. The function is activated.


Once the opening/closing temperatures have been located, the instrument will display the values as *CLOSE* (the closing temperature), *OPEN* (the opening temperature) and *HYSTE*. (the difference between the opening/closing temperatures) respectively. If a temperature has not been found, the instrument will display *Error*.

 To display the three temperatures, press  or .

 Press  to end the test or  to leave the function at any time.

2.8 AUTO STEP

The AUTO STEP function (cf. Fig. 5) is used to step automatically between a range of different set-temperatures.

-  Press . The instrument displays the number of set-temperature **STEPS**.
-  Press  or  to select the required number of steps.
-  Press  to accept your selection. The first set-temperature will flash.
-  Press  or  to select the required temperature.
-  Press  to accept your selection. The next set-temperature will flash. This process will be repeated until the last value has been accepted. The extra **TIME** for which you wish the calibrator to remain at every step will flash.
-  Press  or  to set the required number of minutes.
-  Press  to accept your selection. The function will be activated.
-  Press  after the last set-temperature to end the function or  to leave the function at any time.

2.9 MENU

The MENU function (cf. Fig. 6) is used to modify the SETUP parameters.

 Hold down  for approx. 2 seconds. The word *SETUP* will appear on the display.

 Press . The first SETUP parameter will be displayed.

 Press  or  to toggle between the SETUP parameters:

TEMP. unit: Temperature unit °C or °F.

T-MAX: The highest permissible temperature for the calibrator.

SLOPE rate: Temperature change per minute used in connection with SWITCH TEST.

STABL. Add: Extra time which must elapse once the well is stable before the check mark symbol is displayed.

RESOL: Temperature resolution of 0 or 1 decimal.

 Press  to select the SETUP parameter you wish to change. The current value will flash.

 Press  or  to select the required value.

 Press  to accept your selection or  to cancel and return to the previous value.


 Once you have changed all SETUP parameters as required, cancel the function by pressing  twice.

3.0 Setting the main voltage and replacing the fuses



Warning

- The fuse box must not be removed from the power control switch until the mains cable has been disconnected.
- The two main fuses must be identical and correspond to the chosen voltage.

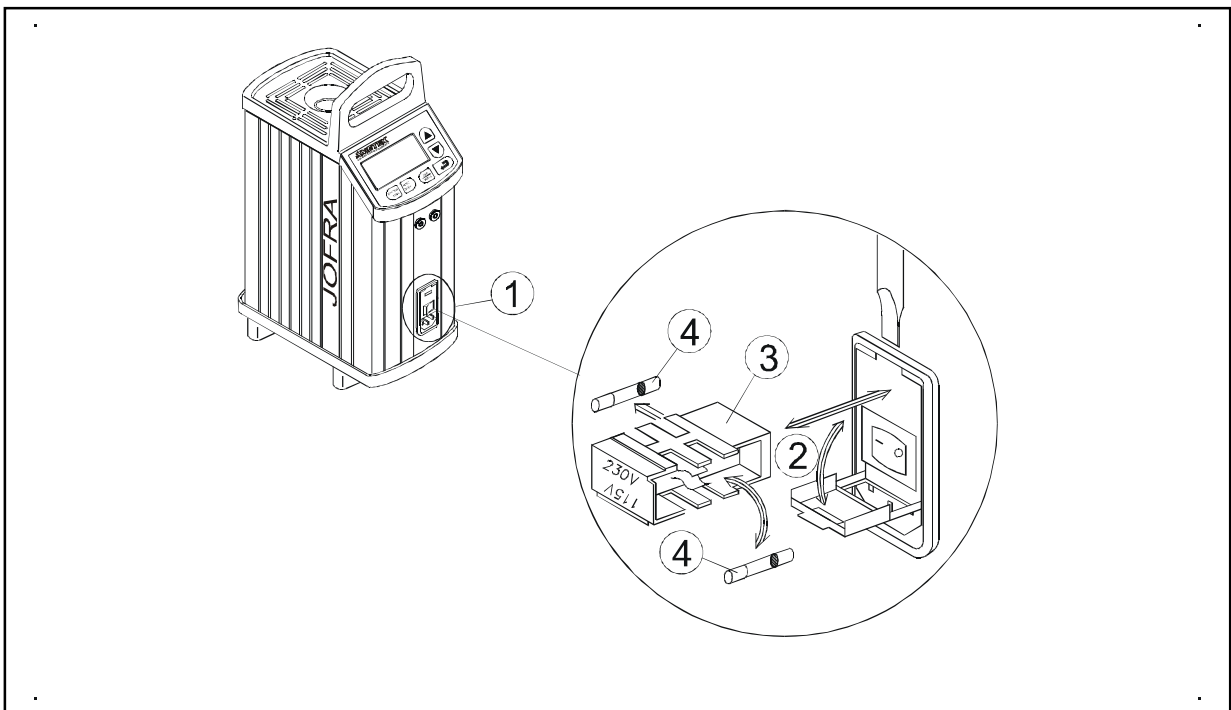

- ① Locate the main fuses in the fuse box in the power control switch and check the voltage of the power control switch (on/off switch (230V/115V)). If the voltage of the power control switch differs from the line voltage, you must adjust the voltage of the power control switch.
- ② Open the lid of the fuse box using a screwdriver.
- ③ Remove the fuse box.
- ④ Remove both fuses and insert two new fuses. These must be identical and should correspond to the line voltage.
 - **ITC-155:** 115V, 2AT = 105014 / 230V, 1AT = 105007

- **ITC-320/650:** 115V, 10AF = 60B302 / 230V, 5AF = 60B301

If the fuses blow immediately after you have replaced them, the calibrator should be returned to the manufacturer for service.

Slide the fuse box into place with the correct voltage turning upwards.

4.0 After use



Warning

Never leave hot insertion tubes which have been removed from the calibrator unsupervised – they may constitute a fire hazard.

If you intend to store the calibrator in the optional carrying case after use, you **must** ensure that the instrument has cooled to a temperature **below 100°C/212°F** before placing it in the carrying case.



Caution...

- The insertion tube must **always** be removed from the calibrator after use.

The humidity in the air may cause verdigris to form on the insertion tube inside the instrument. There is a risk that the insertion tube may become stuck if this is allowed to happen.



Caution – Hot surface

- **Do not touch** the grid plate, the well or the insertion tube - they may be very hot.

The following routine must be observed before the insertion tube is removed and the instrument switched off (cf. Fig. 1):

1. If the calibrator has been heated up to temperatures above 100°C/212°F, you must wait until the instrument reaches a temperature **below 100°C/212°F** before you switch it off.
2. If the calibrator has reached a temperature below 0°C/32°F, it should be heated momentarily to a temperature of 50°C/122°F.
3. Switch off the calibrator using the power control switch (pos. 5).
4. Remove the insertion tube from the calibrator using the tool supplied with the instrument.
5. **Optional:** Store the calibrator in the carrying case.