

Dial Indicator



To ensure operator safety, use this instrument in conformance with the directions and specifications given in this User's Manual. Non-conformance to the instructions may compromise safety.

► Safety Precautions


► Notes on Export Regulations

Do not commit an act which could, directly or indirectly, violate any law or regulation of Japan, your country, or any other international treaty, relating to the export or re-export of any commodities.



KEEP THIS MANUAL FOR FUTURE REFERENCE

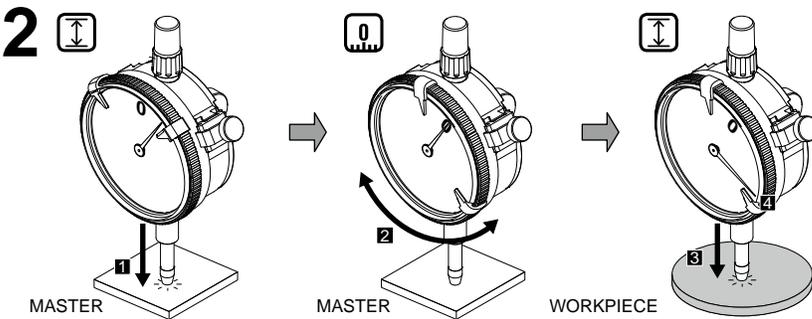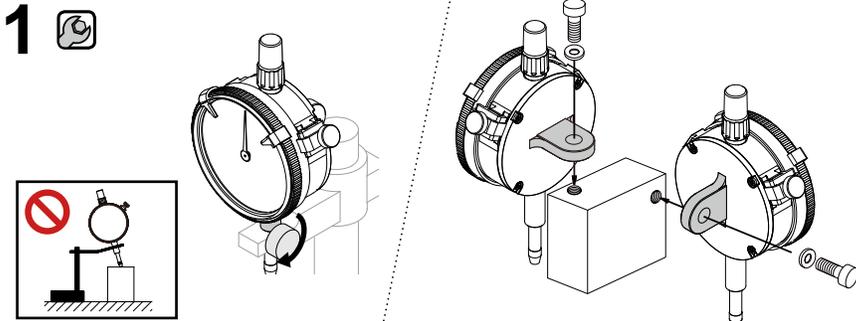

2048A-10,
2048AB-10



2046A-80,
2046AB-80

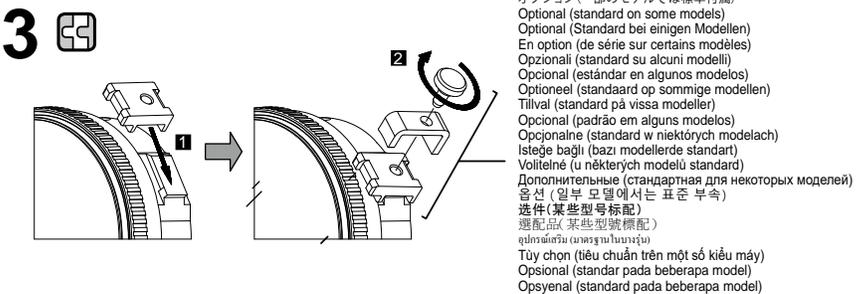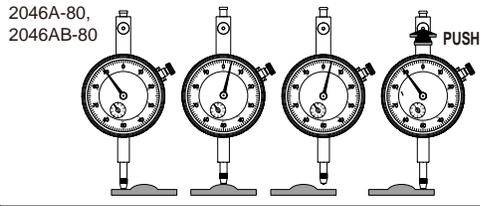

オプション(一部のモデルでは標準付属)
 Optional (standard on some models)
 Optionale (Standard bei einigen Modellen)
 En option (de série sur certains modèles)
 Opzionalni (standard su alcuni modelli)
 Opzionalne (estándar en algunos modelos)
 Opzionale (standaard op sommige modellen)
 Tilval (standard på vissa modeller)
 Opcional (padrão em alguns modelos)
 Opzjonalne (standard w niektórych modelach)
 Istege bağlı (bazı modellerde standart)
 Voitelné (u některých modelů standard)
 Дополнительные (стандартная для некоторых моделей)
 옵션 (일부 모델에서는 표준 부착)
 选项 (某些型号标配)
 選配件 (某些型號標配)
 optionale (standard op sommige modellen)
 Tùy chọn (tiêu chuẩn trên một số kiểu máy)
 Opzional (standar pada beberapa model)
 Opsyenal (standard pada beberapa model)

- Be sure to perform reference point adjustment by following points to notice below.
- Do not perform the adjustment at sites where the temperature will change abruptly. Thermally stabilize the instrument sufficiently at room temperature.
- Wipe oil and dust off the both contact point and master gage using a gauze or chamois skin.
- Perform reference point setting and measurement in the same posture of the product.
- Use a master gage like a setting standard which is periodically calibrated.
- After use, take corrosion prevention measures. Corrosion can cause the caliper to malfunction.

Mitutoyo

Mitutoyo Corporation
 20-1, Sakado 1-chome, Takatsu-Ku,
 Kawasaki-shi, Kanagawa 213-8533, Japan
 Phone:044-813-2330

ONE YEAR WARRANTY

Product Name _____ Code No. _____
 Serial No. _____ Date Purchased _____

Mitutoyo Corporation conducts an own Quality management system based on the requirements of ISO 9001. This product conforms to the Mitutoyo inspection standard, and the standard (s) used for the calibration is /are traceable to the national standard (s).

In the event that this product should fail within one (1) year from the original date of purchase through normal use conforming to the User's Manual provided with the product and Warning Label(s) on the product, we will repair or replace it, our option, free of charge, upon its prepaid return to Mitutoyo with this WARRANTY Card.

► Purchaser is requested to fill the blank above and retain the warranty card at hand. Return card only when requesting Warranty Service.

Y. Takahashi
 Quality Assurance Department
 Y. Takahashi Manager

This warranty shall not apply if the product and consumables have been subject to air wear and tear, abuse through misuse or improper use, handling, storage, maintenance, service, repair or through adaptation/modification by the original purchaser or any third party without prior written consent of Mitutoyo, or as a result of damage by an actual disaster or circumstances beyond the control of Mitutoyo.

To obtain service under this warranty the product must be returned to the retailer you purchased from along with the warranty card. Any postage, insurance, or shipping charges incurred in returning the product for service are the responsibility of the purchaser.

► This warranty is not transferable and is only valid within the country of the original purchase.

► You may have additional rights under the laws of country of original purchase that do not allow the exclusion or limitation of warranties of the exclusion or limitation of certain damages. If these laws apply, Mitutoyo's limitations and exclusions may not apply to you.

