

This low cost, compact indicator is ideally suited for low or high volume applications. The meter features a 9 segment LCD to display 1V d.c. full scale reading. Other voltages and currents can be measured via the addition of 2 scaling resistors. The meter can be used in applications where the order of magnitude of the reading is more important than the value of the reading itself. It allows the operator to scan the display and receive a quick visual feedback. Installation is particularly easy; the module requires only a single round hole in the panel. A rubber seal is included, providing splashproof protection for the unit when fitted to the meter during installation.

- 9 Segment LCD
- **Colour Scale**
- Auto-zero
- 1V d.c. Full Scale Reading
- **Single Hole Mounting**
- **No Calibration Required**
- **Splashproof**

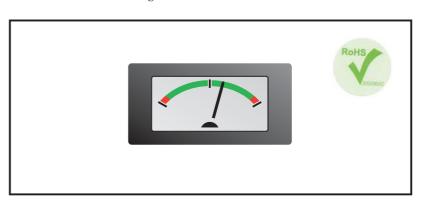

Standard Meter			S	tock Number EMA 1710
Specification	Min.	Тур.	Max.	Unit
Accuracy (overall error) *		1		Segment (<u>+</u> 1)
Full scale reading		1		V d.c.
Resolution		125		mV d.c.
Sample rate		10		samples/sec
Operating temperature range	0		50	°C
Supply voltage (V+ to V-)	5	9	12	V d.c.
Supply current (@5Vd.c.)		6		mA

^{*} At voltages above 1V d.c., the display flashes.

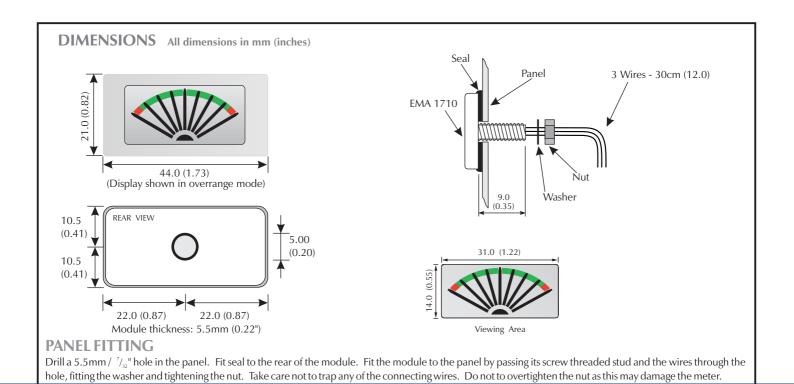

1.888.610.7664



www.calcert.com

sales@calcert.com

WIRE FUNCTIONS


 $Positive\ power\ supply\ connection.$ RED V+**BLACK** 0VNegative power supply connection.

WHITE Vin Positive measuring input with reference to 0V.


Range from 0 to 1V d.c.

SCALING

Two external resistors may be used to alter the full scale reading of the meter - see table for sample values. Alternatively, use the following formulae to calculate Ra and Rb. Select the nearest available standard resistor. To achieve optimum accuracy, use 1% metal film resistors.




Required F.S.R.	Ra	Rb
10V	910k	100k
100V	1M	10k
10mA	0R	100R
100mA	0R	10R



SAFETY

To comply with the Low Voltage Directive (LVD 93/68/EEC), input voltages to the module's pins must not exceed 60Vdc. The user must ensure that the incorporation of the unit into the user's equipment conforms to the relevant sections of BS EN 61010 (Safety Requirements for Electrical Equipment for Measuring, Control and Laboratory Use).

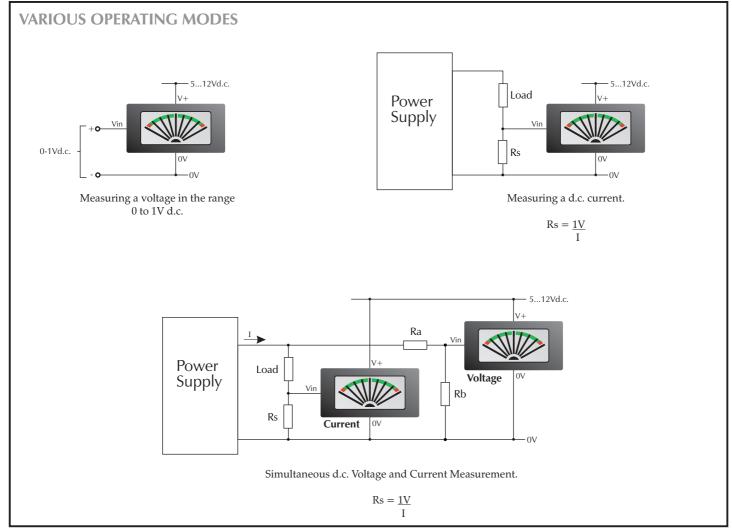

Specifications liable to change without prior warning

EMA 1710

Issue 12

April/2008

IRCN 0539

S.C.

Applies to EMA 1710/2





www.calcert.com

sales@calcert.com