

High-precision, 3-channel power meter with built-in harmonic measurement

Accurately measure devices up to 1000 V/65 A AC/DC with direct input



The PW3336 (2-channel) and PW3337 (3-channel) can measure DC and a variety of power connections ranging from single-phase 2-wire to 3-phase 4-wire*.

- For development and production of motors, inverters, power conditioners, power supplies, and other devices
- Assess and verify the energy-saving performance of industrial equipment such as heavy machinery, air-conditioners as well as household appliances

- | | |
|---|--|
| • Voltage, current, and power basic accuracy | : $\pm 0.1\%$ ** |
| • Measurement frequency bands | : DC, 0.1 Hz to 100 kHz |
| • High-current measurement | : Up to 65 A, direct input |
| • Low-loss current input | : Input resistance of 1m Ω or less |
| • Harmonic measurement up to the 50th order | : IEC 61000-4-7 compliant |
| • High-accuracy measurement, even with a low power factor | : Ideal for no-load testing of transformers and motors |
| • Measure up to 5000 A AC | : Built-in external sensor input terminals |

High-accuracy
High-current
Harmonic measurement

Support for development and production of motors, transformers, air-conditioners, and other industrial equipment



The PW3336 series (2-channel) and PW3337 series (3-channel) are easy-to-use, high-accuracy power meters that deliver current measurement of up to 65 A with direct input as well as built-in harmonic analysis functionality, all with accuracy that exceeds that of previous HIOKI power meters.

World class performance

Measure up to 65 A with direct input

1 Measurement accuracy that remains unchanged for high-current measurement

Accuracy is guaranteed for currents of up to 65 A with direct input. The power meters can also measure high currents in excess of 65 A with optional current sensors. Direct-input power meters typically exhibit degraded accuracy when inputting high currents due to shunt resistor self-heating. However, the PW3336 and PW3337 reduce input resistance with a DCCT design that virtually eliminates this type of accuracy degradation.

2mA	65A	5000A
	Direct input	Sensor input



2 A 3-channel power meter

Enabling you to select the optimal range for each connection. The advanced engineering of the PW3336 and PW3337 enables you to measure an inverter's primary-side DC power supply and its secondary-side 3-phase output at the same time. The power meters make a tremendous contribution in applications that need to measure the input/output efficiency of inverters, uninterruptible power supplies, and other power supply equipment.

Configure multiple ranges with a single instrument



3 Best-in-class accuracy of $\pm 0.1\%$ *

Highest basic accuracy and DC accuracy of any instrument in its class

Thanks to Hioki's accumulated technology and track record, the PW3336/PW3337 delivers the highest basic accuracy and DC accuracy of any instrument in its class. Reliable measurement accuracy ensures robust performance in customers' measurement applications.

$\pm 0.1\%$ *

1.888.610.7664

 www.calcert.com

sales@calcert.com

* For complete details, please refer to the specifications.

Simultaneously measure power consumption and all harmonic parameters, from single-phase 2-wire to 3-phase 4-wire measurement lines

2ch



PW3336 series (2-channel models)
Measurement lines: 1P2W/1P3W/3P3W

3ch




PW3337 series (3-channel models)
Measurement lines: 1P2W/1P3W/3P3W/3P4W

World class performance


4 Simultaneous processing of power data and all harmonic data

All data, including RMS values, mean values, DC components, AC components, fundamental wave components, harmonic measurement, and integration measurement, is processed in parallel internally. There is no need to switch modes depending on whether you wish to acquire power data or harmonic data - simply switch the display to obtain measured values with true simultaneity. Additionally, PC communications software can be used to capture measurement data, including from multiple synchronized instruments.

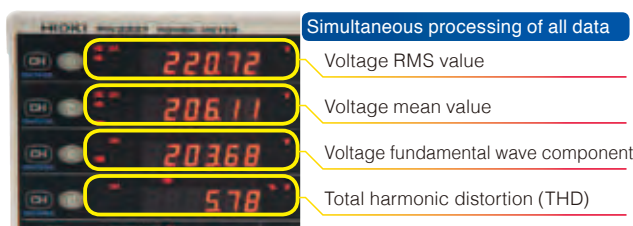

6 Wide frequency band of DC and 0.1 Hz to 100 kHz

Thanks to a wide-band capability extending from DC and 0.1 Hz to 100 kHz, the PW3336/PW3337 can cover not only inverters' fundamental frequency band, but also the carrier frequency band.

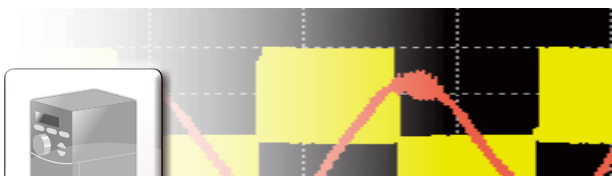

5 High-accuracy measurement, even with low-power-factor input


Because power factor has little impact at just $\pm 0.1\%$ f.s., the PW3336/PW3337 can measure active power of low-power-factor input at a high level of accuracy, for example during no-load-loss testing, a technique that is used to evaluate energy-saving performance of transformers.

Even though the high current waveform crest factor that typically accompanies no-load operation causes the power factor to deteriorate, measurements taken with the PW3336/PW3337 series remain accurate under these conditions.



7 Integrating fluctuating power values

The power consumption of equipment subject to a fluctuating load, for example refrigerators, heaters, and pumps, varies considerably between rated operation and no-load operation. Thanks to its broad dynamic range, the PW3336/PW3337 can perform integrated power measurement with guaranteed accuracy using a single range, even if the power fluctuates dramatically during integration. Measurements can accommodate waveform peaks of up to 600% of the range rating.

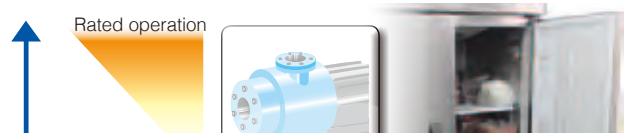

Advanced functions

1 Extensive built-in features including harmonic measurement, current sensor input, synchronized control, and a wide selection of interfaces

The PW3336/PW3337 ships standard with all the functionality you need for measurement. Choose from a total of eight models depending on whether your application requires support for GP-IB communications and D/A output.

Standard functionality by model

● : Built-in function — : Function not available

Model	No. of channels	Harmonic measurement	Current sensor input	Synchronized control	LAN	RS-232C	GP-IB	D/A output
PW3336	2	●	●	●	●	●	—	—
PW3336-01		●	●	●	●	●	●	—
PW3336-02		●	●	●	●	●	—	●
PW3336-03		●	●	●	●	●	●	●
PW3337	3	●	●	●	●	●	—	—
PW3337-01		●	●	●	●	●	●	—
PW3337-02		●	●	●	●	●	—	●
PW3337-03		●	●	●	●	●	●	●

2 IEC61000-4-7 compliant harmonic measurement

The PW3336/PW3337 supports measurement that complies with IEC 61000-4-7:2002, the international standard governing harmonic measurement.

The power meters can measure voltage, current, and power harmonics up to the 50th order depending on the fundamental frequency, including total harmonic distortion (THD), fundamental wave component, harmonic level, phase difference, content percentage, and other parameters for each order. Since you can cap the number of orders for which harmonic analysis is performed to any order from the 2nd to the 50th, you can make standard-compliant calculations, even if the standard defines an upper limit order for THD calculations.

About IEC 61000-4-7

IEC 61000-4-7 is an international standard governing the measurement of harmonic current and harmonic voltage in power supply systems as well as harmonic current emitted from devices. It defines the performance of standard instruments used to make such measurements.

3 Large selection of interfaces

The PW3336/PW3337's interfaces can be used to control the instrument and to capture its data - simply download the free PC application from the HIOKI website. Functionality supported via LAN connections includes power meter configuration, measured value monitoring, waveform monitoring, display of time-series recordings, and capturing data at intervals.



PW3336-03
PW3337-03

4 16-channel D/A output (-02, -03)

D/A output-equipped instruments can generate voltage output for measured values and integrated power with their 16-bit D/A converter. By connecting an external data logger, HIOKI Memory HiCorder, recorder, or other device, you can simultaneously record data along with temperature and other non-power signals. The PW3336/PW3337 also offers the first active power level output on a cycle-by-cycle basis of any instrument in its class.

Three types of D/A output (switchable)

Instantaneous waveform output


Output voltage, current, or power instantaneous waveforms. (Sampling speed: Approx. 87.5 kHz)

Level output

Output voltage, current, power, and other selected parameters with an update cycle of approximately 200 ms.


High-speed active power level output

Generate level output for the active power for each cycle of the measurement waveform.

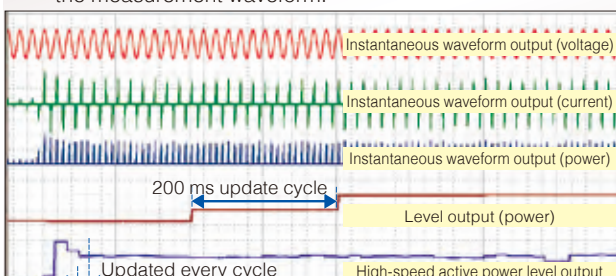


5 Synchronized control using up to 8 instruments

Eight units of PW3336/PW3337 can be connected and their measurements fully synchronized. That means you can have up to 24 channels of simultaneous calculations, display updates, data updates, integration control, display hold timing, and zero-adjustment. In addition, the master-slave configuration allows you to key lock all slave devices with the master unit, mirroring the master unit's operations and modes on all of the other power meters. The free PC application can be used to calculate efficiency values across multiple units.

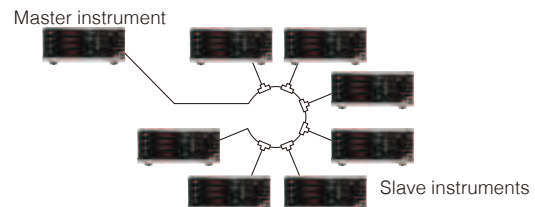

6 Current sensor connectivity

The PW3336/PW3337 can also measure devices that exceed 65 A with the use of an optional current sensor. Measurements with guaranteed accuracy can be performed for currents of up to 5000 A AC. Choose from a range of high-accuracy, clamp or pass-through AC/DC current sensors and models specifically designed for 50/60 Hz measurement.




Applications

1 Research, development, and testing of equipment with 3-phase power supplies such as transformers, motors, air-conditioners, and heavy machinery

Key advantages

- ✓ Measure 3-phase 3-wire and 3-phase 4-wire* lines with a basic measurement accuracy of $\pm 0.1\%$ **
- ✓ Perform high-current measurement of 65 A with direct input without accuracy degradation caused by shunt resistor self-heating.
- ✓ Built-in IEC 61000-4-7 compliant harmonic measurement functionality as well as current sensor input terminals and a LAN interface.
- ✓ Accuracy is guaranteed for active power measurement from 0 W, as well as for measurement of integrated power for loads with large fluctuations.
- ✓ Measure active power at a high level of accuracy even with low power factors, for example during no-load operation testing of transformers.

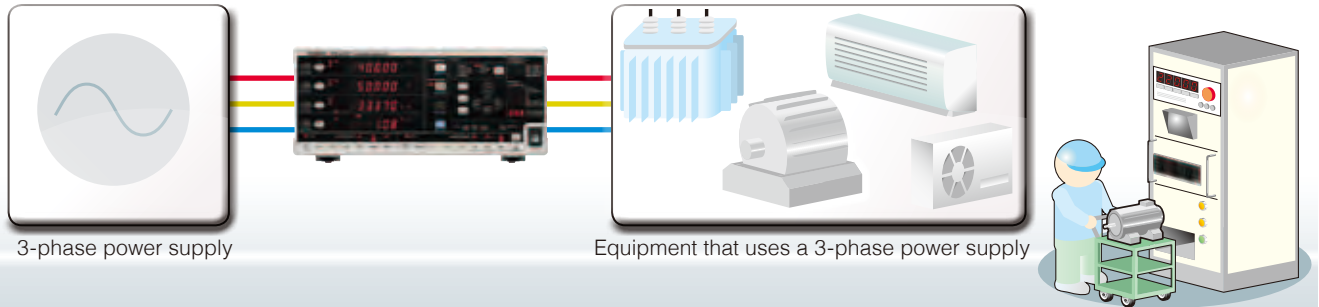


*3-phase 4-wire measurement: PW3337 series only ** For complete details, please refer to the specifications.

2 Measuring the efficiency of power conditioners used in solar power installations

Key advantages

- ✓ Measure primary-side DC and secondary-side 3-phase output with a single PW3337, using the optimal range for each.
- ✓ Calculate efficiency: Perform output/input calculations and easily identify the resulting efficiency on the power meter's screen.
- ✓ Ripple rate calculation: Display the ratio of the AC component that is superposed on a DC line.
- ✓ Built-in current sensor input terminals: Measure currents exceeding 65 A with an optional current sensor.
- ✓ Harmonic measurement: Test for harmonic components such as voltage THD, which can be a concern with grid-linked systems.

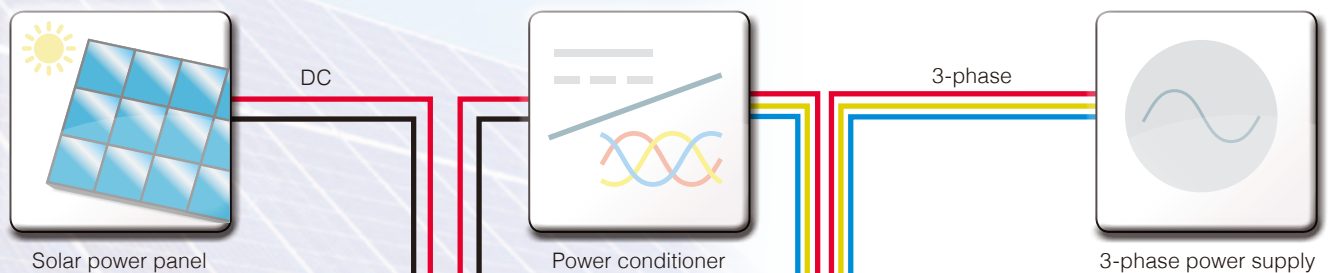


Other DC/3-phase and 1-phase/3-phase measurement applications

- ✓ Measuring the efficiency of battery-powered devices (DC/3-phase) such as electric vehicles
- ✓ Measuring the efficiency of rapid chargers for electric vehicles (3-phase/DC)

3 Measuring power supply devices such as 3-phase/3-phase inverters

Key advantages


- ✓ Connect multiple instruments to synchronize their operation, including display updates, data updates, and start of integration.
- ✓ Measure all data with simultaneous parallel processing, including RMS values, mean values, fundamental wave components, THD, and harmonic components.
- ✓ Wide frequency band from DC and 0.1 Hz to 100 kHz: Enjoy coverage for the inverter secondary-side frequency band.
- ✓ Built-in current sensor input terminals: Measure currents exceeding 65 A with an optional current sensor.

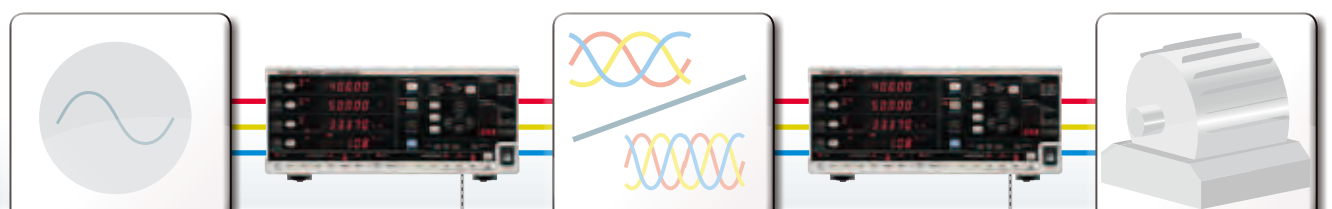

4 Measuring the primary-side, internal circuitry, and secondary-side power consumption in uninterruptible power supplies (UPS)

Key advantages


- ✓ Set individual ranges and measurement types for each channel. Measure power consumption at each stage of the UPS.
- ✓ Hold waveform peak values and measured value maximum and minimum values.
- ✓ Measure all data with simultaneous parallel processing, including RMS values, mean values, fundamental wave components, THD, and harmonic components.

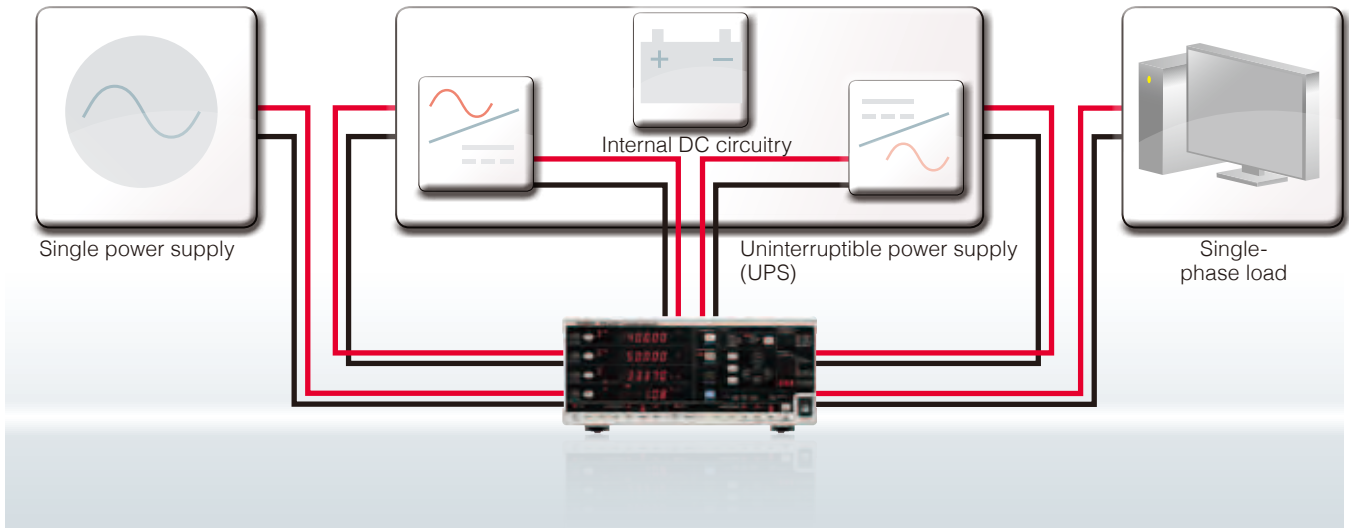

5 Simultaneous measurement of multiple loads

Key advantages

- ✓ Set individual ranges and measurement types for each channel. Measure power consumption at each stage of an uninterruptible power supply.
- ✓ Perform integrated measurement of widely fluctuating power signals without changing the range - useful during long-term integrated power evaluation tests.
- ✓ Use the synchronized control function to sync measurement timing and start/stop integration across a maximum of 8 power meters.

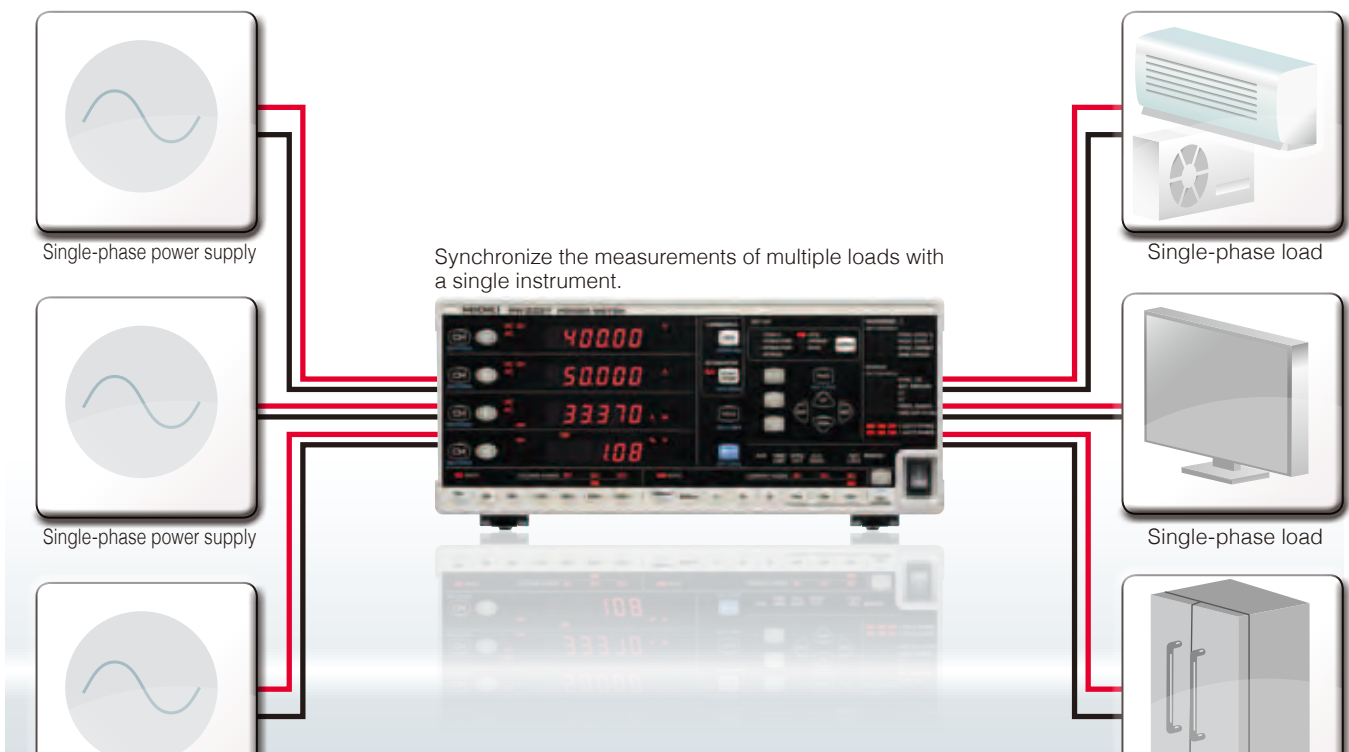

Software

PW3336/PW3337 Communicator

The PW3336/PW3337 Communicator connects with the power meters via the LAN, RS-232C, or GP-IB (-01, -03) interface, and is available for free download from the HIOKI website. Functionality includes configuring instruments, capturing interval data, performing numerical calculations based on measurement data, calculating efficiency values across multiple units, displaying 10 or more measurement parameters, and displaying waveforms.




LabVIEW Driver

Use LabVIEW* to collect data and integrate the power meter into existing systems.

*LabVIEW is a trademark of National Instruments Corporation.

Dimensional drawings

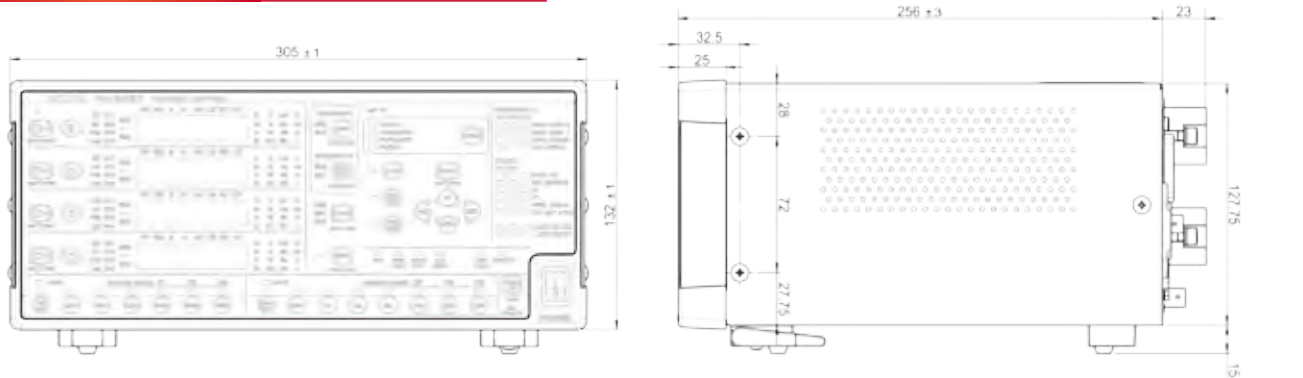

(Unit: mm)

Specifications

Input Specifications

Measurement line type	PW3336 series			
	Single-phase 2-wire (1P2W),			
	Single-phase 3-wire (1P3W),			
	Three-phase 3-wire (3P3W, 3P3W2M)			
	Wiring		CH1	CH2
	1P2W×2		1P2W	1P2W
	1P3W		1P3W	
	3P3W		3P3W	
	3P3W2M		3P3W2M	
	PW3337 series			
Single-phase 2-wire (1P2W),				
Single-phase 3-wire (1P3W),				
Three-phase 3-wire (3P3W, 3P3W2M, 3V3A, 3P3W3M),				
Three-phase 4-wire (3P4W)				

Basic Measurement Specifications

Measurement method	Simultaneous voltage and current digital sampling, zero-cross simultaneous calculation
--------------------	--

Frequency bands	DC, 0.1 Hz to 100 kHz
Synchronization sources	U1, U2, U3, I1, I2, I3, DC (fixed at 200 ms) Can be set separately for each wiring mode.
Measurement items	· Voltage · Current · Active power · Apparent power · Reactive power · Power factor · Phase angle · Frequency · Efficiency · Current integration · Active power integration · Integrated time · Voltage waveform peak value · Current waveform peak value · Voltage crest factor · Current crest factor · Time average current · Time average active power · Voltage ripple factor · Current ripple factor Harmonic parameters: · Harmonic voltage RMS value · Harmonic current RMS value · Harmonic active power · Total harmonic voltage distortion · Total harmonic current distortion · Voltage fundamental waveform · Current fundamental waveform · Active power fundamental waveform · Apparent power fundamental waveform · Reactive power fundamental waveform · Power factor fundamental waveform (displacement power factor) · Voltage current phase difference fundamental waveform · Interchannel voltage fundamental wave phase difference · Interchannel current fundamental wave phase difference · Harmonic voltage content % · Harmonic current content % · Harmonic active power content % The following parameters can be downloaded as data during PC communication but not displayed: · Harmonic voltage phase angle · Harmonic current phase angle · Harmonic voltage current phase difference
Rectifiers	AC+DC : AC+DC measurement Display of true RMS values for both voltage and current AC+DC Umn : AC+DC measurement Display of average value rectified RMS converted values for voltage and true RMS values for current DC : DC measurement Display of simple averages for both voltage and current Display of values calculated by (voltage DC value) × (current DC value) for active power AC : AC measurement Display of values calculated by for both voltage and current Display of values calculated by $\sqrt{(AC+DC \text{ value})^2 - (DC \text{ value})^2}$ for active power FND Extraction and display of the fundamental wave component from harmonic measurement
Zero-Crossing Filter	500 Hz/200 kHz 500 Hz: 0.1 Hz to 500 Hz, 200 kHz: 0.1 Hz to 200 kHz

Measurement accuracy Voltage			
Frequency (f)	Input < 50% f.s.	50% f.s. ≤ Input < 100% f.s.	100% f.s. ≤ Input
DC	±0.1%rdg. ±0.1%f.s.	±0.1%rdg. ±0.1%f.s.	±0.2%rdg.
0.1Hz ≤ f < 16Hz	±0.1%rdg. ±0.2%f.s.	±0.3%rdg.	±0.3%rdg.
16Hz ≤ f < 45Hz	±0.1%rdg. ±0.1%f.s.	±0.2%rdg.	±0.2%rdg.
45Hz ≤ f < 66Hz	±0.1%rdg. ±0.05%f.s.	±0.15%rdg.	±0.15%rdg.
66Hz ≤ f < 500Hz	±0.1%rdg. ±0.1%f.s.	±0.2%rdg.	±0.2%rdg.
500Hz ≤ f < 10kHz	±0.1%rdg. ±0.2%f.s.	±0.3%rdg.	±0.3%rdg.
10kHz ≤ f < 50kHz	±0.5%rdg. ±0.3%f.s.	±0.8%rdg.	±0.8%rdg.
50kHz ≤ f < 100kHz	±2.1%rdg. ±0.3%f.s.	±2.4%rdg.	±2.4%rdg.

Current (direct input)			
Frequency (f)	Input < 50% f.s.	50% f.s. ≤ Input < 100% f.s.	100% f.s. ≤ Input
DC	±0.1%rdg. ±0.1%f.s.	±0.1%rdg. ±0.1%f.s.	±0.2%rdg.
0.1Hz ≤ f < 16Hz	±0.1%rdg. ±0.2%f.s.	±0.3%rdg.	±0.3%rdg.
16Hz ≤ f < 45Hz	±0.1%rdg. ±0.1%f.s.	±0.2%rdg.	±0.2%rdg.
45Hz ≤ f < 66Hz	±0.1%rdg. ±0.05%f.s.	±0.15%rdg.	±0.15%rdg.
66Hz ≤ f < 500Hz	±0.1%rdg. ±0.1%f.s.	±0.2%rdg.	±0.2%rdg.
500Hz ≤ f < 10kHz	±0.1%rdg. ±0.2%f.s.	±0.3%rdg.	±0.3%rdg.
1kHz ≤ f < 10kHz	±(0.03+0.07×F)%rdg. ±0.2%f.s.	±(0.23+0.07×F)%rdg.	±(0.23+0.07×F)%rdg.
10kHz ≤ f < 100kHz	±(0.3+0.04×F)%rdg. ±0.3%f.s.	±(0.6+0.04×F)%rdg.	±(0.6+0.04×F)%rdg.

Active power			
Frequency (f)	Input < 50% f.s.	50% f.s. ≤ Input < 100% f.s.	100% f.s. ≤ Input
DC	±0.1%rdg. ±0.1%f.s.	±0.1%rdg. ±0.1%f.s.	±0.2%rdg.
0.1Hz ≤ f < 16Hz	±0.1%rdg. ±0.2%f.s.	±0.3%rdg.	±0.3%rdg.
16Hz ≤ f < 45Hz	±0.1%rdg. ±0.1%f.s.	±0.2%rdg.	±0.2%rdg.
45Hz ≤ f < 66Hz	±0.1%rdg. ±0.05%f.s.	±0.15%rdg.	±0.15%rdg.
66Hz ≤ f < 500Hz	±0.1%rdg. ±0.1%f.s.	±0.2%rdg.	±0.2%rdg.
500Hz ≤ f < 10kHz	±0.1%rdg. ±0.2%f.s.	±0.3%rdg.	±0.3%rdg.
1kHz ≤ f < 10kHz	±(0.03+0.07×F)%rdg. ±0.2%f.s.	±(0.23+0.07×F)%rdg.	±(0.23+0.07×F)%rdg.
10kHz ≤ f < 50kHz	±(0.07×F)%rdg. ±0.3%f.s.	±(0.3+0.07×F)%rdg.	±(0.3+0.07×F)%rdg.
50kHz ≤ f < 100kHz	±(0.6+0.07×F)%rdg. ±0.3%f.s.	±(0.9+0.07×F)%rdg.	±(0.9+0.07×F)%rdg.

- Values for f.s. depend on measurement ranges.
- "F" in the tables refers to the frequency in kHz.
- Add ±1mA to DC measurement accuracy for current.
- Add (±1mA) × (voltage read value) to DC measurement accuracy for active power.
- When using the 200mA or 500mA range, add ±0.1% rdg. to current and active power for which 1kHz < f ≤ 10kHz.
- Values for voltage, current, and active power for which 0.1Hz ≤ f < 10Hz are for reference only.
- Values for voltage, current, and active power in excess of 220V or 20A for which 10Hz ≤ f < 16Hz are for reference only.
- Values for current and active power in excess of 20A for which 500Hz < f ≤ 50kHz are for reference only.
- Values for current and active power in excess of 15A for which 50kHz < f ≤ 100kHz are for reference only.
- Values for voltage and active power in excess of 750V for which 30kHz < f ≤ 100kHz are for reference only.

Guaranteed accuracy period	1 year
Post-adjustment accuracy guaranteed	6 months
Conditions of guaranteed accuracy	Temperature and humidity : 23°C ±5°C, 80% RH or less Warm-up time : 30 minutes Input : Sine wave input, power factor of 1, terminal-to-ground voltage of 0V, after zero adjustment; within range in which the fundamental wave satisfies synchronization source conditions
Temperature characteristic	±0.03% f.s. per °C or less
Power factor effects	±0.1% f.s. or less (45 to 66 Hz, at power factor = 0) Internal circuitry voltage/current phase difference: ±0.0573°
Effect of common mode voltage	±0.02% f.s. or less (600 V, 50/60 Hz, applied between input terminals and enclosure)
Effect of external magnetic field interference	400 A/m, DC and 50/60 Hz magnetic field Voltage : ±1.5% f.s. or less Current : ±1.5% f.s. or ±10 mA, whichever is greater, or less Active power : ±3.0% f.s. or (voltage influence quantity) × (±10 mA), whichever is greater, or less
Magnetization effect	±10 mA equivalent or less (after inputting 100 A DC to the current direct input terminals)
Adjacent channel input effect	±10 mA equivalent or less (when inputting 50 A to adjacent channel)

Voltage/ Current/ Active Power Measurement Specifications

Measurement types	Rectifiers: AC+DC, DC, AC, FND, AC+DC Umn
Effective measuring range	Voltage : 1% to 130% of range (however, up to ±1500 V peak value and 1000 V RMS value) Current : 1% to 130% of range Active power : 0% to 169% of the range (However, defined when the voltage and current fall within the effective measurement range.)
Display range	Voltage/ Current : 0.5% to 140% of range (zero-suppression when less than 0.5%) Active power : 0% to 196% of the range (no zero-suppression)
Polarity	Voltage/ Current : Displayed when using DC rectifier Active power : +: Positive: Power consumption (no polarity display) -: generation or regenerated power

Voltage/ Current/ Active power channel and sum value calculation formulas

Wiring	X: U (Voltage) or I (Current)	P (Active power)
All channels	1P2W	$X_{(1)}$
	1P3W	
	3P3W	$X_{sum} = \frac{1}{2} (X_{(1)} + X_{(2)})$
	3P3W2M	$P_{sum} = (P_{(1)} + P_{(2)})$

Frequency Measurement Specifications

Number of measurement channels	3
Measurement source	Select from U (VHz) or I (AHz) by channel
Measurement method	Calculated from input waveform period (reciprocal method)
Measurement range	500 Hz/200 kHz (linked to zero-cross filter)
Measurement accuracy	±0.1% rdg. ±1 dgt. (0°C to 40°C)
Effective measuring range	0.1 Hz to 100 kHz For sine wave input that is at least 20% of the measurement source's measurement range. Measurement lower limit frequency setting: 0.1 sec. / 1 sec. / 10 sec.
Display format	0.1000 Hz to 9.9999 Hz, 9.900 Hz to 99.999 Hz, 99.00 Hz to 999.99 Hz, 9900 kHz to 9.9999 kHz, 9.900 kHz to 99.999 kHz, 99.00 kHz to 220.00 kHz

Apparent Power/ Reactive Power/ Power Factor/ Phase Angle Measurement Specifications

Measurement types	Rectifiers Apparent Power/ Reactive Power/ Power Factor: AC+DC, AC, FND, AC+DC Umn Phase Angle : AC, FND
Effective measuring range	As per voltage, current, and active power effective measurement ranges.
Display range	Apparent Power/ Reactive Power : 0% to 196% of the range (no zero-suppression) Power Factor : ±0.0000 to ±1.0000 Phase Angle : +180.00 to -180.00
Polarity	Reactive Power/ Power Factor/ Phase Angle Polarity is assigned according to the lead/lag relationship of the voltage waveform rising edge and the current waveform rising edge. + : When current lags voltage (no polarity display) - : When current leads voltage

Power channel and sum value calculation formulas

Wiring	S : Apparent power	Q : Reactive power
All channels	1P2W $S_{(1)} = U_{(1)} \times I_{(1)}$	$Q_{(1)} = S_{(1)} \sqrt{1 - P_{(1)}^2}$
	1P3W $S_{sum} = S_{(1)} + S_{(2)}$	
	3P3W $S_{sum} = \frac{\sqrt{3}}{2} (S_{(1)} + S_{(2)})$	$Q_{sum} = Q_{(1)} + Q_{(2)}$
	3P3W2M $S_{sum} = \frac{\sqrt{3}}{3} (S_{(1)} + S_{(2)} + S_{(3)})$	
	3V3A $S_{sum} = S_{(1)} + S_{(2)} + S_{(3)}$	$Q_{sum} = Q_{(1)} + Q_{(2)} + Q_{(3)}$
	3P3W3M	
	3P4W	

(i) : Measurement channel

Wiring	λ : Power factor	ϕ : Phase angle
All channels	1P2W $\lambda_{(1)} = \frac{P_{(1)}}{S_{(1)}}$	$\phi_{(1)} = \sin^{-1} I \lambda_{(1)}$
	1P3W	
	3P3W $\lambda_{sum} = \frac{P_{sum}}{S_{sum}}$	When $P_{sum} \geq 0$ $\phi_{sum} = \cos^{-1} \lambda_{sum}$ (0° to ±90°)
	3P3W2M	
	3V3A	When $P_{sum} \geq 0$ $\phi_{sum} = \sin^{-1} 180 - \cos^{-1} \lambda_{sum}$ (±90° to ±180°)
	3P3W3M	
	3P4W	

(i) : Measurement channel ; The polarity symbol λ_{sum} is acquired from the Q_{sum} symbol.

Voltage Waveform Peak Value / Current Waveform Peak Value Measurement Specifications

Measurement method	Measures the waveform's peak value (for both positive and negative polarity) based on sampled instantaneous voltage values.
Sampling frequency	Approx. 700 kHz
Range configuration	
Voltage peak range	
Voltage range	15V 30V 60V 150V 300V 600V 1000V
Voltage peak range	90.000V 180.00V 360.00V 900.00V 1.8000kV 3.6000kV 6.0000kV
Current peak range	
Current range	200mA 500mA 1A 2A 5A 10A 20A 50A
Current peak range	1.2000A 3.0000A 6.0000A 12.000A 30.000A 60.000A 120.00A 300.00A
Measurement accuracy	Same as the voltage or current measurement accuracy at DC and when 10 Hz ≤ f ≤ 1 kHz (f.s.: voltage peak range or current peak range). Provided as reference value when 0.1 Hz ≤ f < 10 Hz and when in excess of 1 kHz.
Effective measuring range	±5% to ±100% of voltage peak range (up to ±1500 V) or ±5% to ±100% of current peak range (up to ±100 A)
Display range	±0.3% to ±102% of voltage peak range or current peak range (values less than ±0.3% are subject to zero-suppression)

Voltage Crest Factor/ Current Crest Factor Measurement Specifications

Measurement method	Calculates values from display values once each display update interval for voltage and voltage waveform peak values or current and current waveform peak values.
Effective measuring range	As per voltage and voltage waveform peak value or current and current waveform peak value effective measurement ranges.
Display range	1.0000 to 612.00 (no polarity)

Synchronized Control

Functions	Timing of calculations, display updates, data updates, integration start/stop/reset events, display hold operation, key lock operation, and zero-adjustment operation for the slave PW3336/PW3337 are synchronized with the master PW3336/PW3337.
Terminal	BNC terminal × 1 (non-isolated)
Terminal name	EXT SYNC
I/O settings	Off: Synchronized control function off In : The EXT SYNC terminal is set to input, and a dedicated synchronization signal can be input (slave). Out: The EXT SYNC terminal is set to output, and a dedicated synchronization signal can be output (master).

Voltage Ripple Rate / Current Ripple Factor Measurement Specifications

Measurement method	Calculates the AC component (peak to peak [peak width]) as a proportion of the voltage or current DC component
Effective measuring range	As per voltage and voltage waveform peak value or current and current waveform peak value effective measurement ranges
Display range	0.00[%] to 500.00[%]
Polarity	None

Efficiency Measurement Specifications

Measurement method	Calculates the efficiency η [%] from the ratio of active power values for channels and wires				
Wiring modes and calculation equations	Calculated based on the AC+DC rectifier active power				
	PW3336 series				
	Wiring (WIRING)	CH1	CH2	Calculation formulas	
	1P2W $\times$ 2	1P2W	1P2W	$\eta_1=100\times P_2 / P_1 $ $\eta_2=100\times P_1 / P_2 $	
	1P3W	1P3W			
	3P3W	3P3W			
	3P3W2M	3P3W2M			
	PW3337 series				
	Wiring (WIRING)	CH1	CH2	CH3	Calculation formulas
	1P2W $\times$ 3	1P2W	1P2W	1P2W	$\eta_1=100\times P_3 / P_1 $ $\eta_2=100\times P_1 / P_3 $
1P3W & 1P2W	1P3W	1P2W		$\eta_1=100\times P_3 / P_{sum} $ $\eta_2=100\times P_{sum} / P_3 $	
3P3W & 1P2W	3P3W	1P2W			
3P3W2M	3P3W2M				
3V3A	3V3A				
3P3W3M	3P3W3M				
3P4W	3P4W				
Effective measuring range	As per the active power effective measurement range.				
Display range	0.00[%] to 200.00[%]				

Functional Specifications

Auto-range (AUTO)	Automatically changes the voltage and current range for each wiring mode according to the input Range up : The range is increased when input exceeds 130% of the range or when the peak is exceeded. Range down : The range is decreased when input falls below 15% of the range. However, the range is not decreased when the peak is exceeded at the lower range.																
Averaging (AVG)	- Averages the voltage, current, active power, apparent power, and reactive power. - The power factor and phase angle are calculated from averaged data. - Measured values other than peak values, power factor, frequency, integrated values, T.AV, crest factor, ripple rate, total harmonic distortion, and harmonics are averaged. Method : Simple averaging Number of averaging iterations and display update interval <table><tr><td>Number of averaging iterations</td><td>1 (OFF)</td><td>2</td><td>5</td><td>10</td><td>25</td><td>50</td><td>100</td></tr><tr><td>Display update interval</td><td>200ms</td><td>400ms</td><td>1s</td><td>2s</td><td>5s</td><td>10s</td><td>20s</td></tr></table>	Number of averaging iterations	1 (OFF)	2	5	10	25	50	100	Display update interval	200ms	400ms	1s	2s	5s	10s	20s
Number of averaging iterations	1 (OFF)	2	5	10	25	50	100										
Display update interval	200ms	400ms	1s	2s	5s	10s	20s										
Scaling (VT, CT)	Applies user-defined VT and CT ratio settings to measured values. These settings can be configured separately for each wiring mode. VT ratio setting range : OFF (1.0), 0.1 to 1000 (setting: 0000) CT ratio setting range : OFF (1.0), 0.001 to 1000 (setting: 0000)																
HOLD (HOLD)	- Stops display updates for all measured values and fixes the display values at that point in time. - Measurement data acquired by communications is also fixed at that point in time. - Internal calculations (including integration and integration elapsed time) will continue. - Analog output and waveform output are not held.																
Maximum value/minimum value hold (MAX/MIN HOLD)	- Detects maximum and minimum measured values as well as maximum and minimum values for the voltage and current waveform peak and holds them on the display. - For data with polarity, display of the maximum value and minimum value for the data's absolute values is held (so that both positive and negative polarity values are shown). - Internal calculations (including integration and integration elapsed time) will continue. - Analog output and waveform output are not held.																
Zero Adjustment (0 ADJ)	Degausses the current input unit DCCT and then zeroes out the current input offset.																
Key-lock (KEY LOCK)	Disables key input in the measurement state, except for the SHIFT key and KEY LOCK key.																
Backup	Backs up settings and integration data if the instrument is turned off and if a power outage occurs.																
System Reset	- Initializes the instrument's settings. - Communications-related settings (communications speed, address, and LAN-related settings) are not initialized.																

Integration Measurement Specifications

Measurement types	Rectifiers: AC+DC, AC+DC Umn Current: Displays the result of integrating current RMS value data (display values) once every display update interval (approx. 200 ms) as an integrated value. Active power: Displays the result of integrating active power values by polarity calculated once every cycle for the selected synchronization source as integrated values. Rectifier: DC
-------------------	---

Integration Measurement Specifications

Measurement items	Simultaneous integration of the following 6 parameters for each channel (total of 18 parameters): - Sum of current integrated values (displayed as Ah on panel display) - Positive current integrated value (displayed as Ah+ on panel display) - Negative current integrated value (displayed as Ah- on panel display) - Sum of active power integrated values (displayed as Wh on panel display) - Positive active power integrated value (displayed as Wh+ on panel display) - Negative active power integrated value (displayed as Wh- on panel display)
Integration time	1 min. to 10000 hr., settable in 1 min. blocks
Integration time accuracy	± 100 ppm ± 1 dgt. (0°C to 40°C)
Integration measurement accuracy	(Current or active power measurement accuracy) + ($\pm 0.01\%$ rdg. ± 1 dgt.)
Effective measuring range	Until PEAK OVER U or PEAK OVER I occurs
Display resolution	999999 (6 digits + decimal point)
Functions	- Stopping integration based on integration time setting (timer) - Displaying the integration elapsed time (displayed as TIME on panel display) - Additional integration by repeatedly starting/stopping integration - Backing up integrated values and the integration elapsed time during power outages - Stopping integration when power returns
External control	Stopping/starting integration and resetting integrated values based on external control
Measuring range	Corresponds to the range set for START integration

Time Average Current / Time Average Active Power Measurement Specifications (T.AV)

Measurement method	Calculates the average by dividing the integrated value by the integration time
Measurement accuracy	$\pm$ (Current or active power measurement accuracy) $\pm$ ($\pm 0.01\%$ rdg. ± 1 dgt.)
Effective measuring range	As per the current or active power effective measurement range

Harmonic Measurement Specifications (built-in function)

Measurement method	- Zero-cross simultaneous calculation method (separate windows by channel according to the wiring mode) - Uniform thinning between zero-cross events after processing with a digital antialiasing filter - Interpolation calculations (Lagrange interpolation) - When the synchronization frequency falls within the 45 Hz to 66 Hz range - IEC 61000-4-7:2002 compliant - Gaps and overlaps may occur if the measurement frequency is not 50 Hz or 60 Hz - When the synchronization frequency falls outside the 45 Hz to 66 Hz range - No gaps or overlap will occur																		
Synchronization source	Conforms to synchronization source (SYNC) for the basic measurement specifications																		
Measurement channels	3																		
Measurement items	<table> <tr> <td> - Harmonic voltage RMS value - Harmonic voltage phase angle - Harmonic current content % - Harmonic current phase angle - Harmonic active power - Harmonic voltage current phase difference - Total harmonic current distortion - Current fundamental waveform - Apparent power fundamental waveform - Power factor fundamental waveform - Voltage current phase difference fundamental waveform - Interchannel voltage fundamental wave phase difference - Interchannel current fundamental wave phase difference </td><td> - Harmonic voltage content % - Harmonic current RMS value - Harmonic current phase angle - Harmonic active power content % - Total harmonic voltage distortion - Voltage fundamental waveform - Active power fundamental waveform - Reactive power fundamental waveform </td></tr> </table> The following parameters can be downloaded as data during PC communication but not displayed: - Harmonic voltage phase angle - Harmonic current phase angle - Harmonic voltage current phase difference	- Harmonic voltage RMS value - Harmonic voltage phase angle - Harmonic current content % - Harmonic current phase angle - Harmonic active power - Harmonic voltage current phase difference - Total harmonic current distortion - Current fundamental waveform - Apparent power fundamental waveform - Power factor fundamental waveform - Voltage current phase difference fundamental waveform - Interchannel voltage fundamental wave phase difference - Interchannel current fundamental wave phase difference	- Harmonic voltage content % - Harmonic current RMS value - Harmonic current phase angle - Harmonic active power content % - Total harmonic voltage distortion - Voltage fundamental waveform - Active power fundamental waveform - Reactive power fundamental waveform																
- Harmonic voltage RMS value - Harmonic voltage phase angle - Harmonic current content % - Harmonic current phase angle - Harmonic active power - Harmonic voltage current phase difference - Total harmonic current distortion - Current fundamental waveform - Apparent power fundamental waveform - Power factor fundamental waveform - Voltage current phase difference fundamental waveform - Interchannel voltage fundamental wave phase difference - Interchannel current fundamental wave phase difference	- Harmonic voltage content % - Harmonic current RMS value - Harmonic current phase angle - Harmonic active power content % - Total harmonic voltage distortion - Voltage fundamental waveform - Active power fundamental waveform - Reactive power fundamental waveform																		
FFT processing word length	32 bits																		
Number of FFT points	4096																		
Window function	Rectangular																		
Analysis window width	<table> <tr> <td>45 Hz $\leq f < 56$ Hz</td><td>178.57 ms to 222.22 ms (10 cycles)</td></tr> <tr> <td>56 Hz $\leq f < 66$ Hz</td><td>181.82 ms to 214.29 ms (12 cycles)</td></tr> <tr> <td>Frequencies other than the above</td><td>185.92 ms to 214.08 ms</td></tr> </table>	45 Hz $\leq f < 56$ Hz	178.57 ms to 222.22 ms (10 cycles)	56 Hz $\leq f < 66$ Hz	181.82 ms to 214.29 ms (12 cycles)	Frequencies other than the above	185.92 ms to 214.08 ms												
45 Hz $\leq f < 56$ Hz	178.57 ms to 222.22 ms (10 cycles)																		
56 Hz $\leq f < 66$ Hz	181.82 ms to 214.29 ms (12 cycles)																		
Frequencies other than the above	185.92 ms to 214.08 ms																		
Data update rate	Depends on window width																		
Synchronization frequency range	10 Hz to 640 Hz																		
Maximum analysis order	<table> <tr> <th>Synchronization frequency (f) range</th><th>Analysis order</th></tr> <tr> <td>10 Hz $\leq f < 45$ Hz</td><td>50th</td></tr> <tr> <td>45 Hz $\leq f < 56$ Hz</td><td>50th</td></tr> <tr> <td>56 Hz $\leq f < 66$ Hz</td><td>50th</td></tr> <tr> <td>66 Hz $\leq f < 100$ Hz</td><td>50th</td></tr> <tr> <td>100 Hz $\leq f < 200$ Hz</td><td>40th</td></tr> <tr> <td>200 Hz $\leq f < 300$ Hz</td><td>25th</td></tr> <tr> <td>300 Hz $\leq f < 500$ Hz</td><td>15th</td></tr> <tr> <td>500 Hz $\leq f < 640$ Hz</td><td>11th</td></tr> </table>	Synchronization frequency (f) range	Analysis order	10 Hz $\leq f < 45$ Hz	50th	45 Hz $\leq f < 56$ Hz	50th	56 Hz $\leq f < 66$ Hz	50th	66 Hz $\leq f < 100$ Hz	50th	100 Hz $\leq f < 200$ Hz	40th	200 Hz $\leq f < 300$ Hz	25th	300 Hz $\leq f < 500$ Hz	15th	500 Hz $\leq f < 640$ Hz	11th
Synchronization frequency (f) range	Analysis order																		
10 Hz $\leq f < 45$ Hz	50th																		
45 Hz $\leq f < 56$ Hz	50th																		
56 Hz $\leq f < 66$ Hz	50th																		
66 Hz $\leq f < 100$ Hz	50th																		
100 Hz $\leq f < 200$ Hz	40th																		
200 Hz $\leq f < 300$ Hz	25th																		
300 Hz $\leq f < 500$ Hz	15th																		
500 Hz $\leq f < 640$ Hz	11th																		
Analysis order upper limit setting	2nd to 50th																		
Measurement accuracy	<table> <tr> <th>Frequency (f)</th><th>Voltage, Current, Active power</th></tr> <tr> <td>DC</td><td>$\pm 0.4\%$rdg. $\pm 0.2\%$f.s.</td></tr> <tr> <td>10 Hz $\leq f < 30$ Hz</td><td>$\pm 0.4\%$rdg. $\pm 0.2\%$f.s.</td></tr> <tr> <td>30 Hz $\leq f < 400$ Hz</td><td>$\pm 0.3\%$rdg. $\pm 0.1\%$f.s.</td></tr> <tr> <td>400 Hz $\leq f < 1$ kHz</td><td>$\pm 0.4\%$rdg. $\pm 0.2\%$f.s.</td></tr> <tr> <td>1 kHz $\leq f < 5$ kHz</td><td>$\pm 1.0\%$rdg. $\pm 0.5\%$f.s.</td></tr> <tr> <td>5 kHz $\leq f < 8$ kHz</td><td>$\pm 4.0\%$rdg. $\pm 1.0\%$f.s.</td></tr> </table> For DC, add ± 1 mA to current and (± 1 mA) $\times$ (voltage read value) to active power.	Frequency (f)	Voltage, Current, Active power	DC	$\pm 0.4\%$ rdg. $\pm 0.2\%$ f.s.	10 Hz $\leq f < 30$ Hz	$\pm 0.4\%$ rdg. $\pm 0.2\%$ f.s.	30 Hz $\leq f < 400$ Hz	$\pm 0.3\%$ rdg. $\pm 0.1\%$ f.s.	400 Hz $\leq f < 1$ kHz	$\pm 0.4\%$ rdg. $\pm 0.2\%$ f.s.	1 kHz $\leq f < 5$ kHz	$\pm 1.0\%$ rdg. $\pm 0.5\%$ f.s.	5 kHz $\leq f < 8$ kHz	$\pm 4.0\%$ rdg. $\pm 1.0\%$ f.s.				
Frequency (f)	Voltage, Current, Active power																		
DC	$\pm 0.4\%$ rdg. $\pm 0.2\%$ f.s.																		
10 Hz $\leq f < 30$ Hz	$\pm 0.4\%$ rdg. $\pm 0.2\%$ f.s.																		
30 Hz $\leq f < 400$ Hz	$\pm 0.3\%$ rdg. $\pm 0.1\%$ f.s.																		
400 Hz $\leq f < 1$ kHz	$\pm 0.4\%$ rdg. $\pm 0.2\%$ f.s.																		
1 kHz $\leq f < 5$ kHz	$\pm 1.0\%$ rdg. $\pm 0.5\%$ f.s.																		
5 kHz $\leq f < 8$ kHz	$\pm 4.0\%$ rdg. $\pm 1.0\%$ f.s.																		

Display Specifications

Display	7-segment LED
Number of display parameters	4

External Current Sensor Input Specifications (built-in feature)

Terminal	Isolated BNC terminals, 1 for each channel																							
Current sensor type switching	Off / Type 1 / Type 2 When set to off, input from the external current sensor input terminal is ignored.																							
Current sensor options	TYPE1 (100 A to 5000 A sensors) 9660, 9661, 9669, CT9667-01/-02/-03 TYPE2 (20 A to 1000 A sensors, Power supply is required to use) CT6862-05, CT6863-05, 9709-05, CT6865-05, 9272-05, CT6841-05, CT6843-05, CT6844-05, CT6845-05, CT6846-05																							
Current measurement range	Auto / 10 A / 20 A / 50 A (range noted on panel) User-selectable for each wiring mode. Can be read directly by manually setting the CT ratio.																							
Power range configuration	Depends on the combination of voltage and current ranges; from 60.000W to 15.000MW (also applies to VA, var)																							
Measurement accuracy																								
Current, Active power																								
Frequency	Input < 50% f.s.	50% f.s. ≤ Input < 100% f.s.	100% f.s. ≤ Input																					
DC	±0.2%rdg. ±0.6% f.s.	±0.2%rdg. ±0.6% f.s.	±0.8%rdg.																					
0.1Hz ≤ f < 16Hz	±0.2%rdg. ±0.2% f.s.	±0.4%rdg.	±0.4%rdg.																					
16Hz ≤ f < 45Hz	±0.2%rdg. ±0.2% f.s.	±0.4%rdg.	±0.4%rdg.																					
45Hz ≤ f ≤ 66Hz	±0.2%rdg. ±0.1% f.s.	±0.3%rdg.	±0.3%rdg.																					
66Hz < f ≤ 500Hz	±0.2%rdg. ±0.2% f.s.	±0.4%rdg.	±0.4%rdg.																					
500Hz < f ≤ 1kHz	±0.2%rdg. ±0.3% f.s.	±0.5%rdg.	±0.5%rdg.																					
1kHz < f ≤ 10kHz	±5.0%rdg.	±5.0%rdg.	±5.0%rdg.																					
10kHz < f ≤ 50kHz																								
50kHz < f ≤ 100kHz																								
	f.s. : Each measurement range •To obtain the current or active power accuracy, add the current sensor's accuracy to the above current and active power accuracy figures. •The effective measurement range and frequency characteristics conform to the current sensor's specifications. •Values for current, and active power for which 0.1 Hz ≤ f < 10 Hz are for reference only. •Values for voltage in excess of 220 V active power for which 10 Hz ≤ f < 16 Hz are for reference only.																							
Temperature characteristics	Current, active power : ±0.08% f.s./°C (instrument temperature coefficient; f.s.: instrument measurement range) Add current sensor temperature coefficient to above.																							
Power factor effects	· Instrument: ±0.15% f.s. or less (45 Hz to 66 Hz with power factor = 0) · Internal circuit voltage/current phase difference: ±0.086° · Add the current sensor phase accuracy to the internal circuit voltage/current phase difference noted above.																							
Current peak value measurement accuracy	· (External current sensor input instrument accuracy) + (±2.0% f.s.) (f.s.:current peak range) · Add the current sensor accuracy to the above.																							
Harmonic measurement accuracy	<table><tr><td>Frequency</td><td>Voltage</td><td>Current, Active power</td></tr><tr><td>DC</td><td>±0.4%rdg. ±0.2% f.s.</td><td>±0.6%rdg. ±0.8% f.s.</td></tr><tr><td>10Hz ≤ f < 30Hz</td><td>±0.4%rdg. ±0.2% f.s.</td><td>±0.6%rdg. ±0.4% f.s.</td></tr><tr><td>30Hz ≤ f ≤ 400Hz</td><td>±0.3%rdg. ±0.1% f.s.</td><td>±0.5%rdg. ±0.3% f.s.</td></tr><tr><td>400Hz < f ≤ 1kHz</td><td>±0.4%rdg. ±0.2% f.s.</td><td>±0.6%rdg. ±0.5% f.s.</td></tr><tr><td>1kHz < f ≤ 5kHz</td><td>±1.0%rdg. ±0.5% f.s.</td><td>±1.0%rdg. ±5.5% f.s.</td></tr><tr><td>5kHz < f ≤ 8kHz</td><td>±4.0%rdg. ±1.0% f.s.</td><td>±2.0%rdg. ±6.0% f.s.</td></tr></table> f.s. : Each measurement range •To obtain the current or active power accuracy, add the current sensor's accuracy to the above current and active power accuracy figures.			Frequency	Voltage	Current, Active power	DC	±0.4%rdg. ±0.2% f.s.	±0.6%rdg. ±0.8% f.s.	10Hz ≤ f < 30Hz	±0.4%rdg. ±0.2% f.s.	±0.6%rdg. ±0.4% f.s.	30Hz ≤ f ≤ 400Hz	±0.3%rdg. ±0.1% f.s.	±0.5%rdg. ±0.3% f.s.	400Hz < f ≤ 1kHz	±0.4%rdg. ±0.2% f.s.	±0.6%rdg. ±0.5% f.s.	1kHz < f ≤ 5kHz	±1.0%rdg. ±0.5% f.s.	±1.0%rdg. ±5.5% f.s.	5kHz < f ≤ 8kHz	±4.0%rdg. ±1.0% f.s.	±2.0%rdg. ±6.0% f.s.
Frequency	Voltage	Current, Active power																						
DC	±0.4%rdg. ±0.2% f.s.	±0.6%rdg. ±0.8% f.s.																						
10Hz ≤ f < 30Hz	±0.4%rdg. ±0.2% f.s.	±0.6%rdg. ±0.4% f.s.																						
30Hz ≤ f ≤ 400Hz	±0.3%rdg. ±0.1% f.s.	±0.5%rdg. ±0.3% f.s.																						
400Hz < f ≤ 1kHz	±0.4%rdg. ±0.2% f.s.	±0.6%rdg. ±0.5% f.s.																						
1kHz < f ≤ 5kHz	±1.0%rdg. ±0.5% f.s.	±1.0%rdg. ±5.5% f.s.																						
5kHz < f ≤ 8kHz	±4.0%rdg. ±1.0% f.s.	±2.0%rdg. ±6.0% f.s.																						

D/A Output Specifications (PW3336-02/-03 and PW3337-02/-03)

Number of output channels	16
Configuration	16-bit D/A converter (polarity + 15 bits)
Output parameters	U1 to U3 (voltage level) or u1 to u3 (instantaneous voltage waveform) (switchable) I1 to I3 (current level) or i1 to i3 (instantaneous current waveform) (switchable) P1 to P3 (active power level) or p1 to p3 (instantaneous power waveform) (switchable) Psum (active power level) or Hi-Psum (high-speed active power level) (switchable) Psum and Hi-Psum output is not available (0 V) when using the 1P2W wiring mode. P12 is output when using 1P3W, 3P3W, or 3P3W2M, and P123 is output when using 3V3A, 3P3W3M, or 3P4W. D/A1 to D/A3 : Select any 3 from channel or sum value for voltage, current, active power, apparent power, reactive power, power factor, phase angle, total harmonic voltage/current distortion, inter-channel voltage/current fundamental wave phase difference, voltage/current crest factor, time average current/active power, voltage/current ripple rate, frequency, efficiency, current integration, active power integration (harmonic output is not available for individual orders). Hi-P1 to Hi-P3 and Hi-Psum (high-speed active power level): Fixed to AC+DC For other level output, select AC+DC, AC+DC Umn, DC, AC, or fnd.
Output accuracy	f.s.: Relative to the output voltage rated value for each output parameter Level output : (Output parameter measurement accuracy) + (±0.2% f.s.) High-speed active power level output : (Output parameter measurement accuracy) + (±0.2% f.s.) Instantaneous waveform output : (Output parameter measurement accuracy) + (±1.0% f.s.)

Output voltage	Level output Voltage, current, active power, apparent power, reactive power, time average current/active power : ±2 V DC for ±100% of range Power factor : ±2 V DC at ±0.0000, 0 V DC at ±1.0000 Phase angle : 0 V DC at 0.00°, ±2 V DC at ±180.00° Voltage/current ripple rate, total harmonic voltage/current distortion : ±2 V DC at 100.00% Voltage/current crest factor : ±2 V DC at 10.000 Frequency : Varies with measured value. +2 V DC per 100 Hz from 0.1000 Hz to 300.00 Hz +2 V DC per 10 kHz from 300.01 Hz to 30,000 kHz +2 V DC per 100 kHz from 30.001 kHz to 220.00 kHz Efficiency : ±2 V DC at 200.00% Current integration, active power integration : ±5 V DC at (range) × (integration set time) Waveform output : 1 V f.s. relative to 100% of range
Maximum output voltage	Approx. ±12 V DC
Output update rate	Level output : Fixed at 200 ms ±50 ms (approx. 5 times per sec.) Update rate is unrelated to number of averaging iterations setting and display hold operation. Waveform output : Approx. 11.4 μs (approx. 87.5 kHz) High-speed P level : Updated once every cycle for the input waveform set as the synchronization source.
Response time	Level output : 0.6 sec. or less (when the input changes abruptly from 0% to 90%, or from 100% to 10%, the time required in order to satisfy the accuracy range) Waveform output : 0.2 ms or less High-speed active power level output : 1 cycle
Temperature characteristic	±0.05% f.s./°C or less
Output resistance	100 Ω ±5 Ω

External control (built-in feature)

Functions	Integration start/stop, integration reset and hold via external control																	
External control	Input signal level: 0 to 5 V (high-speed CMOS level or shorted [Lo]/open [Hi])																	
	<table border="1"> <thead> <tr> <th>Functions</th><th>External control signal</th><th>External control terminal</th></tr> </thead> <tbody> <tr> <td>Start</td><td>Hi → Lo</td><td rowspan="2">START/STOP</td></tr> <tr> <td>Stop</td><td>Lo → Hi</td></tr> <tr> <td>Reset</td><td>Lo interval of at least 200 ms</td><td>RESET</td></tr> <tr> <td>Hold on</td><td>Hi → Lo</td><td rowspan="2">HOLD</td></tr> <tr> <td>Hold off</td><td>Lo → Hi</td></tr> </tbody> </table>	Functions	External control signal	External control terminal	Start	Hi → Lo	START/STOP	Stop	Lo → Hi	Reset	Lo interval of at least 200 ms	RESET	Hold on	Hi → Lo	HOLD	Hold off	Lo → Hi	
Functions	External control signal	External control terminal																
Start	Hi → Lo	START/STOP																
Stop	Lo → Hi																	
Reset	Lo interval of at least 200 ms	RESET																
Hold on	Hi → Lo	HOLD																
Hold off	Lo → Hi																	

GP-IB interface (PW3336-01/-03, PW3337-01/-03)

Method	IEEE488.1 1978 compliant; see IEEE488.2 1987 Interface functions: SH1, AH1, T6, L4, SR1, RL1, PP0, DC1, DT1, C0 Remote control by controller
Address	00 to 30

RS-232C interface (built-in feature)

Connector	D-sub 9-pin connector × 1
Communication method	Full duplex, Start-stop synchronization, Stop bits: 1 (fixed), Data bits: 8 (fixed), Parity: None Remote control by controller
Communication Speed	9600bps/ 38400bps

LAN interface (built-in feature)

Connector	RJ-45 connector × 1
Electrical Specifications	IEEE802.3 compliant
Transmission Method	10BASE-T/100BASE-TX (automatic detection)
Protocol	TCP/IP
Functions	HTTP server (remote operation, firmware updates) Dedicated ports (command control, data transfer) Remote control by controller (REMOTE lamp will light up.)

General Specifications (product guaranteed for one year)

Operating environment	Indoors, altitude up to 2000 m (6562-ft.), pollution degree 2
Operating temperature and humidity	0 to 40°C (32 to 104°F), 80% RH or less (non-condensating)
Storage temperature and humidity	-10 to 50°C (14 to 122°F) 80% RH or less (non-condensating)
Dielectric strength	4290 Vrms AC (sensed current: 1 mA) Between voltage input terminals and (case, interface, and output terminals) Between current direct input terminals and (case, interface, and output terminals) Between voltage input terminals and current direct input terminals
Maximum rated voltage to earth	Voltage input terminal, Current direct input terminal Measurement category III 600 V (anticipated transient overvoltage 6000 V) Measurement category II 1000 V (anticipated transient overvoltage 6000 V)
Maximum input voltage	Between voltage input terminals U: 1000 V, ±1500 V peak
Maximum input current	Between +/- current direct input terminals I: ±70 A, ±100 A peak
Applicable Standards	Safety : EN61010, EMC : EN61326 Class A/ EN61000-3-2/ EN61000-3-3
Rated supply voltage	100 VAC to 240 VAC, Rated power supply frequency : 50/60 Hz
Maximum rated power	40 VA or less
Dimensions	Approx. 305W(12.01") × 132H(5.20") × 256D(10.08") mm (excluding protrusions)

Current Measurement Options [Type 1] Specifications (Can be connected to the current sensor input terminals on the PW3336/PW3337 series.)

Model	CLAMP ON SENSOR 9660	CLAMP ON SENSOR 9661	CLAMP ON SENSOR 9669	FLEXIBLE CLAMP ON SENSOR CT9667-01	FLEXIBLE CLAMP ON SENSOR CT9667-02	FLEXIBLE CLAMP ON SENSOR CT9667-03
Appearance						
Primary current rating	100A AC	500A AC	1000 A AC	500A/ 5000A AC		
Measurable conductor diameter	Max. ϕ 15mm (0.59")	Max. ϕ 46mm (1.81")	Max. ϕ 55 mm (2.17"), 80 (3.15") $\times$ 20(0.79") mm busbar	Max. ϕ 100mm (3.94")	Max. ϕ 180mm (7.09")	Max. ϕ 254mm (10.0")
Basic accuracy	$\pm 0.3\%$ rdg. $\pm 0.02\%$ f.s. (amplitude) $\pm 1^\circ$ or less (phase) (At 45 Hz to 66 Hz)	$\pm 0.3\%$ rdg. $\pm 0.01\%$ f.s. (amplitude) $\pm 0.5^\circ$ or less (phase) (At 45 Hz to 66 Hz)	$\pm 1.0\%$ rdg. $\pm 0.01\%$ f.s. (amplitude) $\pm 1^\circ$ or less (phase) (At 45 Hz to 66 Hz)	$\pm 2.0\%$ rdg. $\pm 0.3\%$ f.s. (amplitude) $\pm 1^\circ$ or less (At 45 Hz to 66 Hz)		
Frequency characteristics	$\pm 1.0\%$ or less (At 40Hz to 5kHz)			$\pm 3\text{dB}$ or less (At 10 Hz to 20kHz)		
Operating Temperature	0 to 50°C (32 to 122°F)			-25 to 65°C (-13 to 149°F)		-10 to 50°C (14 to 122°F)
Effect of conductor position	Within $\pm 0.5\%$ (deviation from center)			Within $\pm 3\%$ (deviation from center)		
Effect of external electromagnetic field	0.1A equivalent or lower (400A/m, 55Hz)			1.5% f.s. or lower (400A/m, 55Hz)		
Maximum rated voltage to earth	CAT III 300Vrms			CATIII 1000 Vrms, CATIV 600 Vrms		
Dimensions	46W(1.81") $\times$ 135H(5.31") $\times$ 21D(0.83")mm Cable length: 3 m (9.84 ft)	78W(3.07") $\times$ 152H(5.98") $\times$ 42D(1.65")mm Cable length: 3 m (9.84 ft)	99.5W(3.92") $\times$ 188H(7.40") $\times$ 42D(1.65") mm Cable length: 3 m (9.84 ft)	Circuit box: 35W (1.38") $\times$ 120.5H (4.74") $\times$ 34D (1.34") mm, Cable length: 2m (between flexible loop and circuit box), 1m (output cable)		
Mass	230g(8.1oz.)	380g(13.4oz.)	590g (20.8 oz.)	280 g (9.9oz.)	280 g (9.9oz.)	470 g (4.9 oz.)
Power supply	—			LR6 alkaline battery x2, or AC Adapter 9445-02/ 9445-03 (sold separately)		

Current Measurement Options [Type 2] Specifications (Requires Sensor Unit CT9555 or CT9557, and Connection Cable L9217.)

Model	AC/DC CURRENT PROBE CT6841-05	AC/DC CURRENT PROBE CT6843-05	AC/DC CURRENT PROBE CT6844-05	AC/DC CURRENT PROBE CT6845-05	AC/DC CURRENT PROBE CT6846-05
Appearance					
Rated primary current	20 A AC/DC	200 A AC/DC	500 A AC/DC	500 A AC/DC	1000 A AC/DC
Frequency band	DC to 1 MHz	DC to 500 kHz	DC to 200 kHz	DC to 100 kHz	DC to 20 kHz
Diameter of measurable conductors	Max. ϕ 20 mm (0.79") (insulated conductor)	Max. ϕ 20 mm (0.79") (insulated conductor)	Max. ϕ 20 mm (0.79") (insulated conductor)	Max. ϕ 50 mm (1.97") (insulated conductor)	Max. ϕ 50 mm (1.97") (insulated conductor)
Basic accuracy (At DC)	$\pm 0.3\%$ rdg. $\pm 0.05\%$ f.s. (amplitude)	$\pm 0.3\%$ rdg. $\pm 0.02\%$ f.s. (amplitude)	$\pm 0.3\%$ rdg. $\pm 0.02\%$ f.s. (amplitude)	$\pm 0.3\%$ rdg. $\pm 0.02\%$ f.s. (amplitude)	$\pm 0.3\%$ rdg. $\pm 0.02\%$ f.s. (amplitude)
Basic accuracy (At DC < f $\leq$ 100 Hz)	$\pm 0.3\%$ rdg. $\pm 0.01\%$ f.s. (amplitude) $\pm 0.1^\circ$ (phase)	$\pm 0.3\%$ rdg. $\pm 0.01\%$ f.s. (amplitude) $\pm 0.1^\circ$ (phase)	$\pm 0.3\%$ rdg. $\pm 0.01\%$ f.s. (amplitude) $\pm 0.1^\circ$ (phase)	$\pm 0.3\%$ rdg. $\pm 0.01\%$ f.s. (amplitude) $\pm 0.1^\circ$ (phase)	$\pm 0.3\%$ rdg. $\pm 0.01\%$ f.s. (amplitude) $\pm 0.1^\circ$ (phase)
Frequency characteristics (Amplitude)	to 500 Hz: $\pm 0.3\%$ rdg. $\pm 0.02\%$ f.s. to 1 kHz: $\pm 0.5\%$ rdg. $\pm 0.02\%$ f.s. to 10 kHz: $\pm 1.5\%$ rdg. $\pm 0.02\%$ f.s. to 100 kHz: $\pm 5.0\%$ rdg. $\pm 0.05\%$ f.s. to 1 MHz: $\pm 30\%$ rdg. $\pm 0.05\%$ f.s. (Includes derating characteristics)	to 500 Hz: $\pm 0.3\%$ rdg. $\pm 0.02\%$ f.s. to 1 kHz: $\pm 0.5\%$ rdg. $\pm 0.02\%$ f.s. to 10 kHz: $\pm 1.5\%$ rdg. $\pm 0.02\%$ f.s. to 50 kHz: $\pm 5.0\%$ rdg. $\pm 0.02\%$ f.s. to 500 kHz: $\pm 30\%$ rdg. $\pm 0.05\%$ f.s. (Includes derating characteristics)	to 500 Hz: $\pm 0.3\%$ rdg. $\pm 0.02\%$ f.s. to 1 kHz: $\pm 0.5\%$ rdg. $\pm 0.02\%$ f.s. to 10 kHz: $\pm 1.5\%$ rdg. $\pm 0.02\%$ f.s. to 50 kHz: $\pm 5.0\%$ rdg. $\pm 0.02\%$ f.s. to 200 kHz: $\pm 30\%$ rdg. $\pm 0.05\%$ f.s. (Includes derating characteristics)	to 500 Hz: $\pm 0.3\%$ rdg. $\pm 0.02\%$ f.s. to 1 kHz: $\pm 0.5\%$ rdg. $\pm 0.02\%$ f.s. to 10 kHz: $\pm 1.5\%$ rdg. $\pm 0.02\%$ f.s. to 20 kHz: $\pm 5.0\%$ rdg. $\pm 0.02\%$ f.s. to 100 kHz: $\pm 30\%$ rdg. $\pm 0.05\%$ f.s. (Includes derating characteristics)	to 500 Hz: $\pm 0.5\%$ rdg. $\pm 0.02\%$ f.s. to 1 kHz: $\pm 1.0\%$ rdg. $\pm 0.02\%$ f.s. to 5 kHz: $\pm 2.0\%$ rdg. $\pm 0.02\%$ f.s. to 10 kHz: $\pm 5.0\%$ rdg. $\pm 0.05\%$ f.s. to 20 kHz: $\pm 30\%$ rdg. $\pm 0.10\%$ f.s. (Includes derating characteristics)
Operating Temperature	-40°C to 85°C (-40°F to 185°F)	-40°C to 85°C (-40°F to 185°F)	-40°C to 85°C (-40°F to 185°F)	-40°C to 85°C (-40°F to 185°F)	-40°C to 85°C (-40°F to 185°F)
Effect of conductor position	Within $\pm 0.1\%$ rdg. (DC to 100 Hz)	Within $\pm 0.1\%$ rdg. (DC to 100 Hz)	Within $\pm 0.1\%$ rdg. (DC to 100 Hz)	Within $\pm 0.2\%$ rdg. (DC to 100 Hz)	Within $\pm 0.2\%$ rdg. (50/60 Hz)
Effect of external magnetic fields	50 mA equivalent or lower (400 A/m, 60 Hz and DC)	50 mA equivalent or lower (400 A/m, 60 Hz and DC)	100 mA equivalent or lower (400 A/m, 60 Hz and DC)	150 mA equivalent or lower (400 A/m, 60 Hz and DC)	150 mA equivalent or lower (400 A/m, 60 Hz and DC)
Dimensions	153W (6.02") $\times$ 67H (2.64") $\times$ 25D (0.98") mm Cable length: 3 m (9.84 ft)	153W (6.02") $\times$ 67H (2.64") $\times$ 25D (0.98") mm Cable length: 3 m (9.84 ft)	153 (6.02") W $\times$ 67 (2.64") H $\times$ 25 (0.98") D mm Cable length: 3 m (9.84 ft)	238 (9.37") W $\times$ 116 (4.57") H $\times$ 35 (1.38") D mm Cable length: 3 m (9.84 ft)	238 (9.37") W $\times$ 116 (4.57") H $\times$ 35 (1.38") D mm Cable length: 3 m (9.84 ft)
Mass	350 g (12.3 oz)	370 g (13.1 oz)	400 g (14.1 oz)	860 g (30.3 oz)	990 g (34.9)
Power supply	SENSOR UNIT CT9555 or CT9557	SENSOR UNIT CT9555 or CT9557	SENSOR UNIT CT9555 or CT9557	SENSOR UNIT CT9555 or CT9557	SENSOR UNIT CT9555 or CT9557


Model	AC/DC CURRENT SENSOR CT6862-05	AC/DC CURRENT SENSOR CT6863-05	AC/DC CURRENT SENSOR 9709-05	AC/DC CURRENT SENSOR CT6865-05	CLAMP ON SENSOR 9272-05
Appearance					
Rated primary current	50 A AC/DC	200 A AC/DC	500 A AC/DC	1000 A AC/DC	20A/200A AC
Frequency band	DC to 1 MHz	DC to 500 kHz	DC to 100 kHz	DC to 20 kHz	1 Hz to 100 kHz
Diameter of measurable conductors	Max. ϕ 24mm (0.94")	Max. ϕ 24 mm (0.94")	Max. ϕ 36 mm (1.42")	Max. ϕ 36 mm (1.42")	Max. ϕ 46mm (1.81")
Basic accuracy	$\pm 0.05\%$ rdg. $\pm 0.01\%$ f.s. (amplitude) $\pm 0.2^\circ$ (phase, not defined for DC) (At DC and 16 Hz to 400 Hz)	$\pm 0.05\%$ rdg. $\pm 0.01\%$ f.s. (amplitude) $\pm 0.2^\circ$ (phase, not defined for DC) (At DC and 16 Hz to 400 Hz)	$\pm 0.05\%$ rdg. $\pm 0.01\%$ f.s. (amplitude) $\pm 0.2^\circ$ (phase, not defined for DC) (At DC and 45 Hz to 66 Hz)	$\pm 0.05\%$ rdg. $\pm 0.01\%$ f.s. (amplitude) $\pm 0.2^\circ$ (phase, not defined for DC) (At DC and 16 Hz to 66 Hz)	$\pm 0.3\%$ rdg. $\pm 0.01\%$ f.s. (amplitude) $\pm 0.2^\circ$ (phase) (At 45 Hz to 66 Hz)
Frequency characteristics (Amplitude)	to 16 Hz: $\pm 0.1\%$ rdg. $\pm 0.02\%$ f.s. 400Hz to 1kHz: $\pm 0.2\%$ rdg. $\pm 0.02\%$ f.s. to 50 kHz: $\pm 1.0\%$ rdg. $\pm 0.02\%$ f.s. to 100 kHz: $\pm 2.0\%$ rdg. $\pm 0.05\%$ f.s. to 1 MHz: $\pm 30\%$ rdg. $\pm 0.05\%$ f.s. (Includes derating characteristics)	to 16 Hz: $\pm 0.1\%$ rdg. $\pm 0.02\%$ f.s. 400Hz to 1kHz: $\pm 0.2\%$ rdg. $\pm 0.02\%$ f.s. to 10 kHz: $\pm 1.0\%$ rdg. $\pm 0.02\%$ f.s. to 100 kHz: $\pm 5.0\%$ rdg. $\pm 0.05\%$ f.s. to 500 kHz: $\pm 30\%$ rdg. $\pm 0.05\%$ f.s. (Includes derating characteristics)	to 45 Hz: $\pm 0.2\%$ rdg. $\pm 0.02\%$ f.s. 66 Hz to 500 Hz: $\pm 0.2\%$ rdg. $\pm 0.02\%$ f.s. to 5 kHz: $\pm 0.5\%$ rdg. $\pm 0.05\%$ f.s. to 10 kHz: $\pm 5.0\%$ rdg. $\pm 0.10\%$ f.s. to 100 kHz: $\pm 30\%$ rdg. $\pm 0.10\%$ f.s. (Includes derating characteristics)	to 16 Hz: $\pm 0.1\%$ rdg. $\pm 0.02\%$ f.s. 66 Hz to 100 Hz: $\pm 0.5\%$ rdg. $\pm 0.02\%$ f.s. to 500 Hz: $\pm 1.0\%$ rdg. $\pm 0.02\%$ f.s. to 5 kHz: $\pm 5.0\%$ rdg. $\pm 0.05\%$ f.s. to 20 kHz: $\pm 30\%$ rdg. $\pm 0.1\%$ f.s. (Includes derating characteristics)	1 Hz to 10 Hz: $\pm 2.0\%$ rdg. $\pm 0.10\%$ f.s. to 45 Hz: $\pm 0.5\%$ rdg. $\pm 0.02\%$ f.s. 66 Hz to 5 kHz: $\pm 1.0\%$ rdg. $\pm 0.05\%$ f.s. to 50 kHz: $\pm 5.0\%$ rdg. $\pm 0.10\%$ f.s. to 100 kHz: $\pm 30\%$ rdg. $\pm 0.10\%$ f.s. (Includes derating characteristics)
Operating Temperature	-30°C to 85°C (-22°F to 185°F)	-30°C to 85°C (-22°F to 185°F)	0°C to 50°C (32°F to 122°F)	-30°C to 85°C (-22°F to 185°F)	0°C to 50°C (-32°F to 122°F)
Effect of conductor position	Within $\pm 0.01\%$ rdg. (DC to 100 Hz)	Within $\pm 0.01\%$ rdg. (DC to 100 Hz)	Within $\pm 0.05\%$ rdg. (DC)	Within $\pm 0.05\%$ rdg. (50/60 Hz)	Within $\pm 0.2\%$ rdg. (55Hz)
Effect of external magnetic fields	10 mA equivalent or lower (400 A/m, 60 Hz and DC)	50 mA equivalent or lower (400 A/m, 60 Hz and DC)	50 mA equivalent or lower (400 A/m, 60 Hz and DC)	200 mA equivalent or lower (400 A/m, 60 Hz and DC)	100 mA equivalent or lower (400 A/m, 60 Hz)
Dimensions	70W (2.76") $\times$ 100H (3.94") $\times$ 53D (2.09") mm Cable length: 3 m (9.84 ft)		160W (6.30") $\times$ 112H (4.41") $\times$ 50D (1.97") mm Cable length: 3 m (9.84 ft)		78W(3.07") $\times$ 188H(7.40") $\times$ 35D(1.38")mm Cable length: 3 m (9.84 ft)
Mass	340 g (12.0 oz.)	350 g (12.3 oz.)	850 g (30.0 oz.)	980 g (35.3 oz)	430g (15.2 oz.)
Power supply	SENSOR UNIT CT9555 or CT9557	SENSOR UNIT CT9555 or CT9557	SENSOR UNIT CT9555 or CT9557	SENSOR UNIT CT9555 or CT9557	SENSOR UNIT CT9555 or CT9557

Type 2 Current Sensor Options

	SENSOR UNIT CT9555	SENSOR UNIT CT9557
Appearance		
Number of available sensors	1	4 With additive output function

	Connection Cord L9217
Appearance	

Type 2 Current Sensor Connection Diagram

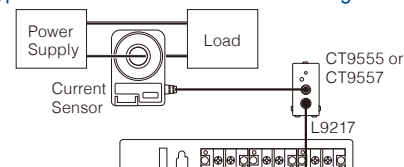

Model : POWER METER PW3336



Model No. (Order Code) (Note)

PW3336	(2ch)
PW3336-01	(2ch, with GP-IB)
PW3336-02	(2ch, with D/A output)
PW3336-03	(2ch, with GP-IB, D/A output)

Accessories: Instruction manual ×1, Measurement guide ×1, Power cord ×1

Model : POWER METER PW3337



Model No. (Order Code) (Note)

PW3337	(3ch)
PW3337-01	(3ch, with GP-IB)
PW3337-02	(3ch, with D/A output)
PW3337-03	(3ch, with GP-IB, D/A output)

Accessories: Instruction manual ×1, Measurement guide ×1, Power cord ×1

Options

Current measurement options [Type 1] Can be directly connected to the current sensor input terminals on the PW3336/ PW3337 series



CLAMP ON SENSOR 9660
100 A AC, $\phi 15$ mm (0.59"), 40 Hz to 5 kHz
 $\pm 0.3\%$ rdg $\pm 0.02\%$ f.s. (Amplitude accuracy 45 Hz to 66 Hz)
 $\pm 1^\circ$ or less (Phase accuracy 45 Hz to 66 Hz)

CLAMP ON SENSOR 9661
500 A AC, $\phi 46$ mm (1.81"), 40 Hz to 5 kHz
 $\pm 0.3\%$ rdg $\pm 0.01\%$ f.s. (Amplitude accuracy 45 Hz to 66 Hz)
 $\pm 0.5^\circ$ or less (Phase accuracy 45 Hz to 66 Hz)



CLAMP ON SENSOR 9669
1000 A AC, $\phi 55$ mm (2.17"), 80×20 mm (3.15" $\times$ 0.79") busbar, 40 Hz to 5 kHz
 $\pm 1.0\%$ rdg $\pm 0.01\%$ f.s. (Amplitude accuracy 45 Hz to 66 Hz)
 $\pm 1^\circ$ or less (Phase accuracy 45 Hz to 66 Hz)

CLAMP ON SENSOR CT9667-01, CT9667-02, CT9667-03
500 A / 5000 A AC Switchable, $\phi 100$ mm to $\phi 254$ mm (3.94" to 10"), 10 Hz to 20 kHz
 $\pm 2.0\%$ rdg $\pm 0.3\%$ f.s. (Amplitude accuracy 45 Hz to 66 Hz)
 $\pm 1^\circ$ or less (Phase accuracy 45 Hz to 66 Hz)
Power supply : LR6 alkaline battery $\times 2$, or AC Adapter (option)
Option : AC ADAPTER 9445-02 (universal 100 V to 240 VAC /for USA)
AC ADAPTER 9445-03 (universal 100 V to 240 VAC /for Europe)

Current measurement options [Type 2] Requires SENSOR UNIT CT9555 or CT9557, and CONNECTION CORD L9217 to be connected to the current sensor input terminals on the PW3336/ PW3337 series

200 A or lower



AC/DC CURRENT SENSOR CT6862-05
50 A AC/DC, pass-through type, $\phi 24$ mm (0.94"), DC to 1 MHz
 $\pm 0.05\%$ rdg $\pm 0.01\%$ f.s. (Amplitude accuracy 16 Hz to 400 Hz)
 $\pm 0.2^\circ$ or less (Phase accuracy 16 Hz to 400 Hz)
Power supply : SENSOR UNIT CT9555 or CT9557 (option)



AC/DC CURRENT SENSOR CT6863-05
200 A AC/DC, pass-through type, $\phi 24$ mm (0.94"), DC to 500 kHz
 $\pm 0.05\%$ rdg $\pm 0.01\%$ f.s. (Amplitude accuracy 16 Hz to 400 Hz)
 $\pm 0.2^\circ$ or less (Phase accuracy 16 Hz to 400 Hz)
Power supply : SENSOR UNIT CT9555 or CT9557 (option)



AC/DC CURRENT PROBE CT6841-05
20 A AC/DC, clamp-on type, $\phi 20$ mm (0.79"), DC to 1 MHz
 $\pm 0.3\%$ rdg $\pm 0.01\%$ f.s. (Amplitude accuracy DC $< f \leq 100$ Hz)
 $\pm 0.1^\circ$ or less (Phase accuracy DC $< f \leq 100$ Hz)
Power supply : SENSOR UNIT CT9555 or CT9557 (option)



AC/DC CURRENT PROBE CT6843-05
200 A AC/DC, clamp-on type, $\phi 20$ mm (0.79"), DC to 500 kHz
 $\pm 0.3\%$ rdg $\pm 0.01\%$ f.s. (Amplitude accuracy DC $< f \leq 100$ Hz)
 $\pm 0.1^\circ$ or less (Phase accuracy DC $< f \leq 100$ Hz)
Power supply : SENSOR UNIT CT9555 or CT9557 (option)



CLAMP ON SENSOR 9272-05 (Scheduled for release in 2017)
20 A / 200 A AC Switchable, clamp-on type, $\phi 46$ mm (1.81"), 1 Hz to 100 kHz
 $\pm 0.3\%$ rdg $\pm 0.01\%$ f.s. (Amplitude accuracy 45 Hz to 66 Hz)
 $\pm 0.2^\circ$ or less (Phase accuracy 45 Hz to 66 Hz)
Power supply : SENSOR UNIT CT9555 or CT9557 (option)

500 A or lower



AC/DC CURRENT SENSOR 9709-05
500 A AC/DC, pass-through type, $\phi 36$ mm (1.42"), DC to 100 kHz
 $\pm 0.05\%$ rdg $\pm 0.01\%$ f.s. (Amplitude accuracy 45 Hz to 66 Hz)
 $\pm 0.2^\circ$ or less (Phase accuracy 45 Hz to 66 Hz)
Power supply : SENSOR UNIT CT9555 or CT9557 (option)



AC/DC CURRENT PROBE CT6844-05
500 A AC/DC, clamp-on type, $\phi 20$ mm (0.79"), DC to 200 kHz
 $\pm 0.3\%$ rdg $\pm 0.01\%$ f.s. (Amplitude accuracy DC $< f \leq 100$ Hz)
 $\pm 0.1^\circ$ or less (Phase accuracy DC $< f \leq 100$ Hz)
Power supply : SENSOR UNIT CT9555 or CT9557 (option)



AC/DC CURRENT PROBE CT6845-05
500 A AC/DC, clamp-on type, $\phi 50$ mm (1.97"), DC to 100 kHz
 $\pm 0.3\%$ rdg $\pm 0.01\%$ f.s. (Amplitude accuracy DC $< f \leq 100$ Hz)
 $\pm 0.1^\circ$ or less (Phase accuracy DC $< f \leq 100$ Hz)
Power supply : SENSOR UNIT CT9555 or CT9557 (option)

1000 A or lower



AC/DC CURRENT SENSOR CT6865-05
1000 A AC/DC, pass-through type, $\phi 36$ mm (1.42"), DC to 20 kHz
 $\pm 0.05\%$ rdg $\pm 0.01\%$ f.s. (Amplitude accuracy 16 Hz to 66 Hz)
 $\pm 0.2^\circ$ or less (Phase accuracy 16 Hz to 66 Hz)
Power supply : SENSOR UNIT CT9555 or CT9557 (option)



AC/DC CURRENT PROBE CT6846-05
1000 A AC/DC, clamp-on type, $\phi 50$ mm (1.97"), DC to 20 kHz
 $\pm 0.3\%$ rdg $\pm 0.01\%$ f.s. (Amplitude accuracy DC $< f \leq 100$ Hz)
 $\pm 0.1^\circ$ or less (Phase accuracy DC $< f \leq 100$ Hz)
Power supply : SENSOR UNIT CT9555 or CT9557 (option)

Type 2 Current sensor options



SENSOR UNIT CT9555
Power supply :
100 V to 240 V AC (50Hz/ 60Hz)



SENSOR UNIT CT9557
Four Sensors can be used.
With additive output function
Power supply : 100 V to 240 V AC (50Hz/ 60Hz)



CONNECTION CORD L9217
For sensor output,
Isolated BNC to isolated BNC
Cord length: 1.6 m (5.25 ft) length

Communications and control options



RS-232C CABLE 9637
Cable length: 1.8 m (5.91 ft)
9pin to 9pin



RS-232C CABLE 9638
Cable length: 1.8 m (5.91 ft)
9pin to 25pin



GP-IB CONNECTOR CABLE 9151-02
Cable length: 2 m (6.56 ft)



LAN CABLE 9642
Cable length: 5 m (16.41 ft)
supplied with straight to cross conversion cable



CONNECTION CORD 9165
For synchronized control
Cable length: 1.5 m (4.92 ft),
metal BNC to metal BNC

Note: Company names and Product names appearing in this catalog are trademarks or registered trademarks of various companies.

HIOKI
HIOKI E. E. CORPORATION



www.calcert.com

sales@calcert.com