




## User Manual

# Digi-Sense® TC9100 Advanced PID and On/Off Temperature Controller with Thermocouple Input

Models 89800-11 and 89800-12

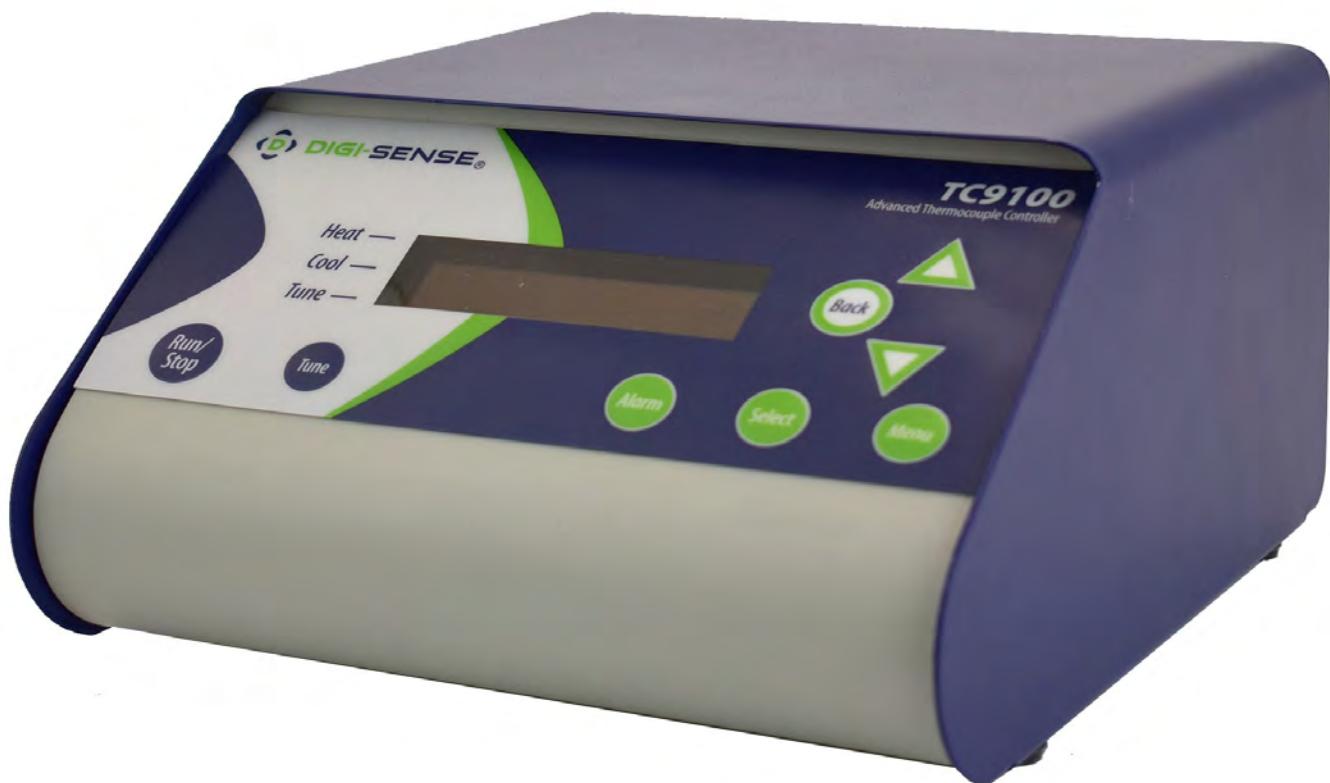

THE STANDARD IN PRECISION MEASUREMENT



## Table of Contents

Introduction .....	3
Unpacking .....	3
Controller Description—Front Panel .....	4
Controller Description—Back Panel.....	5
Controller Description—Active Display Screen .....	6
Setup and Operation .....	7
Initial Setup .....	7
Basic Operation Setup.....	7
Auto Tune Setup.....	7
PID Control Mode Setup (Default Mode) .....	8–15
ON/OFF Control Mode Setup .....	16–22
Safety .....	23
Specifications for Controller Models .....	24
Specifications for Sensor Input .....	25
Screen Flow Charts .....	26–27
General Setup Flow Chart .....	26
Advanced Menu Setup Flow Chart .....	27
Ferrite Clip Installation.....	28
Alternative Power Cords—for Various Countries .....	29
Output Cord Adapters—for Various Countries .....	30
Approvals .....	31
Maintenance.....	32

## Introduction

The Digi-Sense TC9100 Advanced PID and On/Off Temperature Controller (Models 89800-11 and 89800-12) is designed to regulate a user-defined output device at a set point temperature. The microprocessor control uses a PID algorithm that provides precise heating/cooling tolerances for demanding applications in the laboratory or industrial setting.

The TC9100 is a microprocessor-based, digital indicating, single-loop temperature controller. It has a single output located on the back of the controller. It features an auto-tuning function that allows automatic configuration of the PID parameters with minimum user configuration required. The TC9100 has a single thermocouple input that accepts J, K, N, R, S, T, B, and E sensors.


The controller automatically sets the PID parameters through a "learning" sequence in the auto tune mode. PID parameters include proportional band, reset/integral, and rate/derivative. The user-friendly LED display is to aid in monitoring and setup of the controller. The controller automatically stores all user-defined information in nonvolatile memory.

## Unpacking

Check individual parts against the list of items below. If anything is missing or damaged, please contact your instrument supplier immediately.

1. Temperature controller
2. Grid support bracket (attached to the back of the controller)
3. 6-ft (3-m) detachable IEC power cord. Model 89800-11 comes standard with a US 120 VAC plug; Model 89800-12 comes standard with a US 220 VAC plug. See page 32 for additional cords.
4. Electrical noise canceling ferrite clip (connects to sensor input; see page 31 for reference)
5. User manual
6. Quick-start guide

# Controller Description — Front Panel

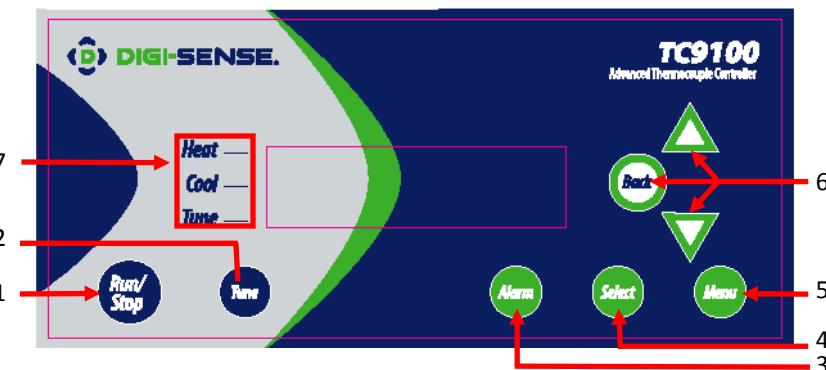

## 1. RUN/STOP Button

Pressing RUN/STOP once will start the control process if the temperature Controller is stopped, or stop the control process if the temperature controller is running. If the controller is running, "Heat" and "Cool" on-screen indicators will illuminate appropriately in the "Alarm/Action Display".

## 2. TUNE Button

Pressing TUNE once will start the AUTO TUNE cycle. AUTO TUNING must be enabled in the setup mode for this key to function. (See page 14, Screen 16)

## 3. ALARM Button

In an ALARM situation, the screen will display either "WARNING" or "ERROR" with the corresponding message. A "WARNING" will not stop the control process. An "ERROR" will stop the control process.

**A. MANUAL RESET mode:** Pressing ALARM once will silence the audible alarm and clear the on-screen alarm message. If the alarm situation is still present, the "Alarm/Action Display" will remain illuminated. The alarm and on-screen message will not clear automatically, even if the system is no longer in an alarm situation.

**B. AUTO RESET mode:** Pressing ALARM once will silence the audible alarm and clear the on-screen alarm message. If the alarm situation is still present, the "Alarm/Action Display" will remain illuminated. If the system leaves an alarm situation, the system will automatically silence the alarm and clear the on-screen alarm message.

## 4. SELECT Button

Pressing SELECT once will cycle through user-configurable control set points. All user-configurable set points will be underlined with a greyed out line. The selected set point will be underlined. Change the set point with the UP and DOWN arrow buttons.

## 5. MENU Button

The MENU button provides access to all user-configurable setup parameters of the controller. Pressing this key once will scroll through parameter options. Pressing and holding this key will exit to the home screen, saving any changes made up to that point.

## 6. UP, DOWN, BACK Buttons

The UP and DOWN arrow buttons will increase or decrease the value of the set point selected (underlined). Pressing the UP or DOWN arrow keys will increase or decrease *numerical* entries by the least significant digit. The rate of acceleration will increase as shown in the table below, starting from the least significant digit. Pressing and holding the UP or DOWN arrow key will increase or decrease *text* entries without an acceleration factor. The Back button moves backwards through the General and Advanced Setup Menus. To exit to the main screen from either menu, press and hold the MENU button.


Numbers...	Increase/Decrease by...
0.0 – 0.9	0.1
0 – 9	1
10 – 100	10
100 +	50

Table 1. Acceleration Factor Table

## 7. HEAT, COOL, AND TUNE Indicators

When any of these modes are active they will have a block indicator on the display showing they are active. **Example:** When the controller is in the heat mode and it is applying power to the heater output there will be an indicator block on the display to show the heater output is active.

## Controller Description — Back Panel

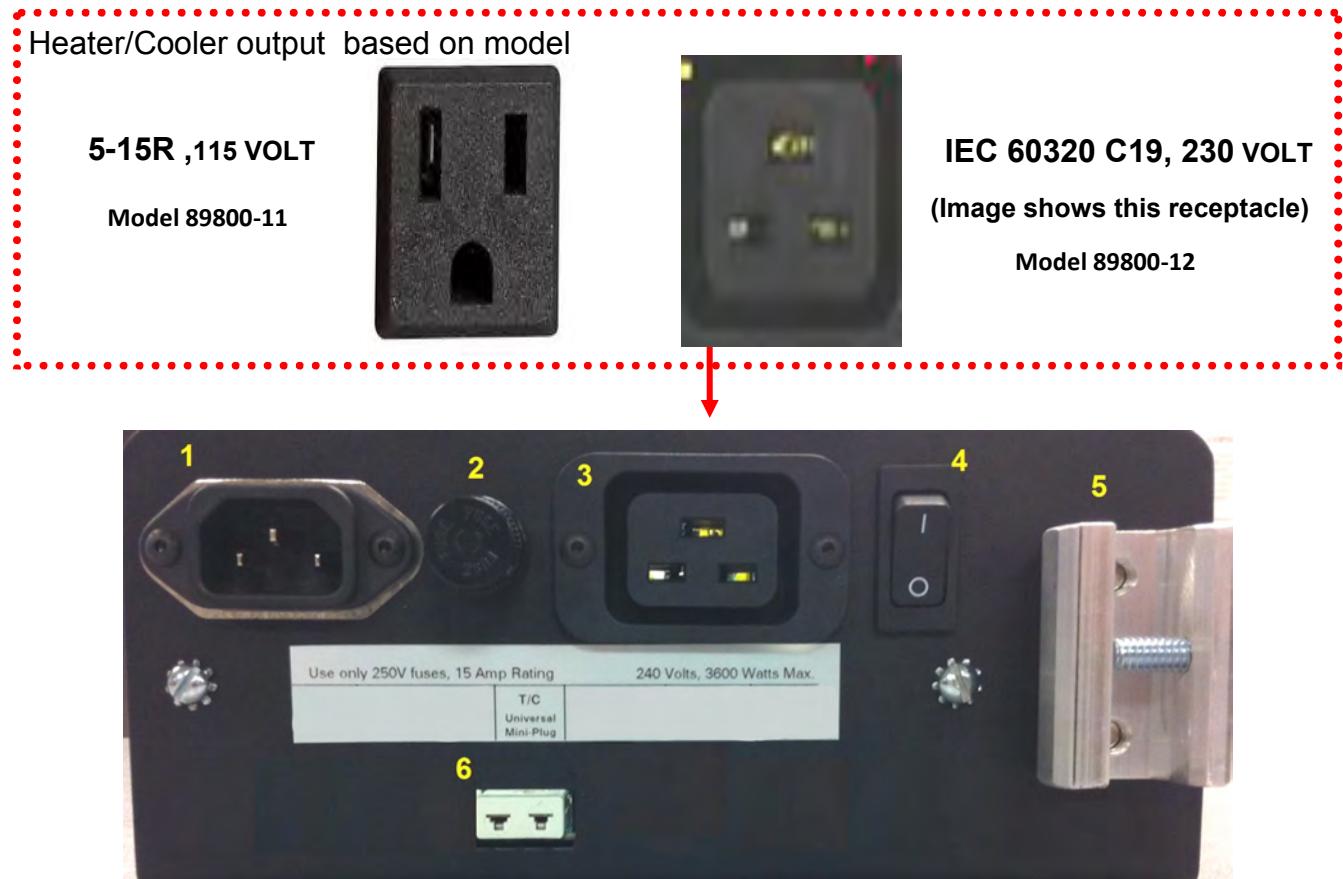

1. IEC power cord connection (see page 32 for additional cords)
2. Fuse
3. Heater/cooling output (see pages 33-34 for optional output cord adapters dependent on country)
4. Power switch
5. Grid support bracket
6. Thermocouple input (accepts type J, K, N, R, S, T, B, and E with mini-connector)

## Controller Description — Active Display Screen

editable value


static text

greyscale Text


situational text

TEXT EXPLANATION

### MAIN SCREENS

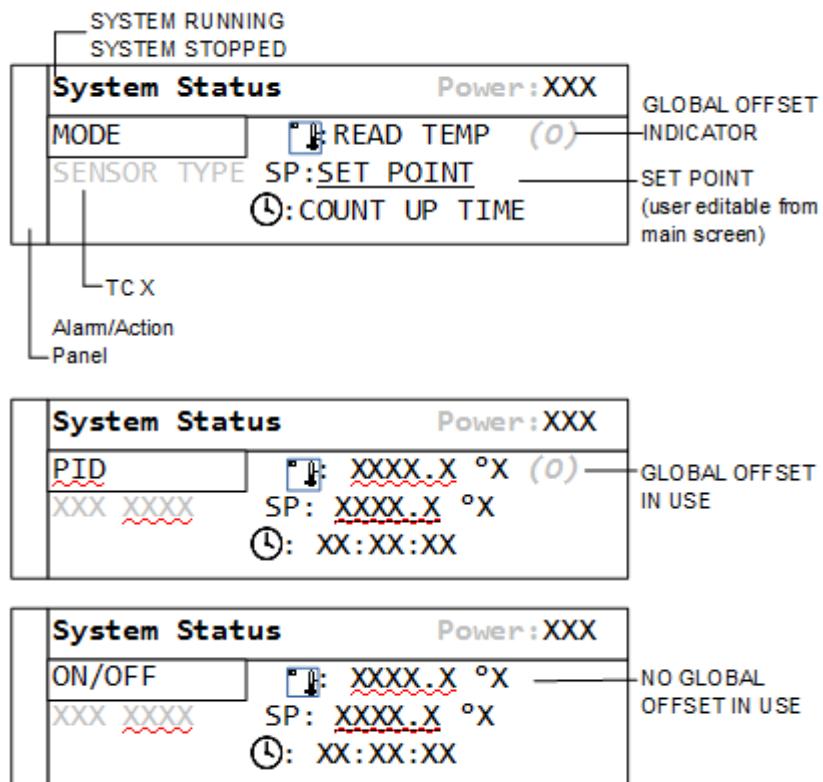

### ALARM ACTION PANEL

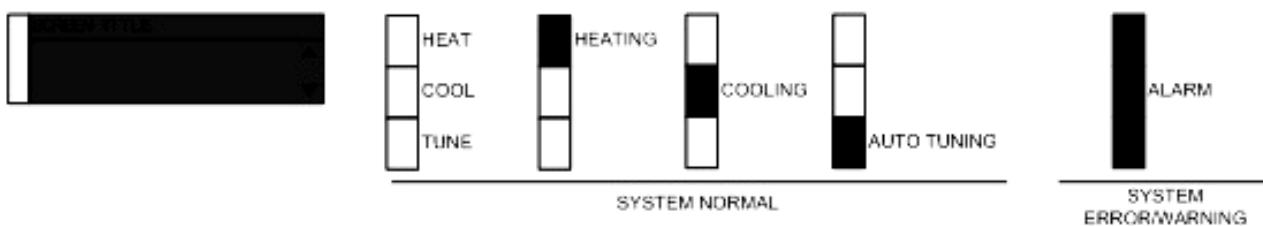

### NAVIGATION



# Setup and Operation

## **Initial Setup**

- Install controller in safe operating area.
- Plug the heater or cooler (sold separately) into the output connector located on the back of the controller.
- Connect the thermocouple sensor to the thermocouple input connector located on the back of the controller.
- Place the ferrite clip over the lead wire of the thermocouple sensor. (See page 28 for reference picture of installation of ferrite clip.)
- Plug the supplied AC cord into the IEC power connector located on the back of the controller.

## **Basic Operation Setup**

- Turn power switch ON, located on the back of controller.
- Follow the instructions on the “welcome” screen.
  - Press SELECT key to read a brief description of each key on the front of controller.
  - Press the MENU key to skip the instructions and enter the main operation screen.
- Press the SELECT key to make a user-editable field active. A line will appear under the field when the field is active for editing.
- Use the UP/DOWN arrow keys to adjust the value that is active in a user-editable field.
- Enter the user-configurable setup by pressing the MENU key from the system status screen.
- Use the MENU key to advance through each menu setting.
- Hold UP and press DOWN arrow keys to jump directly to Output Power adjustment screen.
- Depending on process operation, follow the directions to set up the controller for the proper operation of your process:
  - PID (Factory default) on pages 8-15
  - ON/OFF on pages 16-22
- All changed settings will be retained in memory when returning to the System Status screen.
- Use the flow charts (see pages 26-27) to have a visual of the controls menu layout.


## **Auto Tune Setup**

- Set up your process as noted in the initial setup.
- Verify that the Auto Tune feature is enabled in the menu settings.
- From the main operation screen, set the set point temperature.
- Press the TUNE button and the indicators showing Heat and Tune will be illuminated on display.
- The Set Point value can not be altered after the Tune process has started. The value is locked until the Tune process is complete or aborted by the user.
- Please note that the controller will tune at 90% of the set point. Don't be alarmed if the controller does not reach your entered set point in the tune mode.
- Stopping the Tune operation prior to it finishing will cause the PID settings to be returned to factory default values.

## **PID Control Mode Setup: (FACTORY DEFAULT MODE)**


### **Screen # 1 - Selecting Sensor Type**

- The TC9100 is set to thermocouple.
- Press MENU key to advance to next screen.

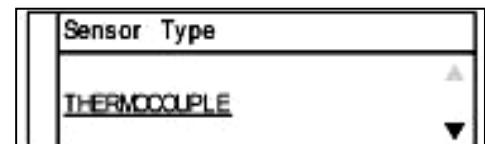

### **Screen # 2 - Selecting Thermocouple Type**

- Thermocouple is preselected on screen # 1.
- Use the UP/DOWN arrow keys to select the desired thermocouple type: J, K, N, R, S, T, B, or E.
- Press MENU key to advance to screen # 3 after selection has been made.

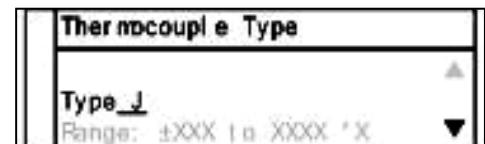

### **Screen # 3 - Selecting Temperature Scale**

- Use the UP/DOWN keys to select the desired temperature scale: Celsius °C, Fahrenheit °F, Kelvin K, Reaumur °Ré, or Rankine °Ra.
- Press MENU key to advance to screen # 4 after selection has been made.



## PID Control Mode Setup:

### **Screen # 4 - Selecting Alarm Setting**



- Use the UP/DOWN arrow keys to change between Auto Reset, Manual Reset, and Off.
- Press MENU key to advance to next screen.
  - If Auto or Manual is selected, the controller will advance to screen # 5.
  - If selection is OFF, the controller will advance to screen # 9.

### **Screen # 5 - Selecting Alarm Mode**



- Use the UP/DOWN arrow keys to select alarm mode.
- Selectable alarm modes:
  - **Process High:** The alarm will be activated if the temperature rises above the user set alarm value.
  - **Process Low:** The alarm will be activated if the temperature goes below the user set alarm value.
  - **Process High/Low:** The alarm will be activated if the temperature goes above or below the high and low temperature levels set by user.
- Press the MENU key to advance to screen # 6 after selecting alarm mode.

## **PID Control Mode Setup:**

### **Screen # 6 - Setting Alarm Mode Variables**

- This screen reflects the variable settings for the selected alarm mode from screen # 5.

#### **- Set Point—Process High**

- Press the UP/DOWN arrow keys to adjust the temperature value.
- When complete, press MENU key to advance to screen # 7.

Alarm Mode
PROCESS HIGH

#### **- Set Point—Process Low**

- Press the UP/DOWN arrow keys to adjust the temperature value.
- When complete, press MENU key to advance to screen # 7.

Process Low
LOW <u>XXXX_X</u> °X

#### **- Set Point—Process High/Low**

- Press the UP/DOWN arrow keys to adjust the temperature value.
- Press the SELECT key to toggle between High and Low. There will be a line below the active field.
- When complete, press MENU key to advance to screen # 7.

Process High/ Low
High: <u>XXXX_X</u> °X
Low: <u>XXXX_X</u> °X

## PID Control Mode Setup:

### **Screen # 7 - Setting Hysteresis Alarm**

- Use the UP/DOWN arrow keys to adjust value.
- The user-defined value when the alarm will exit an alarm condition. **Example:** User has a Process High alarm programmed with a value of 150°C and has set the Alarm Hysteresis of 1°C. The alarm has been activated after the temperature reached 160°C. When temperature reaches 149°C, the alarm condition will not be active.
- When complete, press MENU key to advance to screen # 8.




### **Screen # 8 - Setting Audible Alarm**

- Use UP/DOWN arrow keys to change value to either ON audible alarm or OFF audible alarm.
- When complete, press MENU key to advance to screen # 9.



### **Screen # 9 - Advanced Menu Gateway**

- Use the UP/DOWN arrow keys to change selection to ENTER.
- When complete, press MENU key to advance to screen # 10.
- The following screens are in the advanced portion of the setup menu:

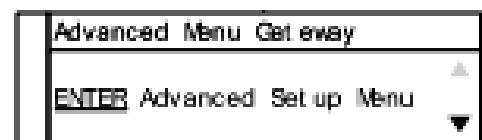

**Screen # 10 - Calibration Gateway**

**Screen # 11 - Global Sensor Offset**

**Screen # 12 - Over Temperature Stop**

**Screen # 13 - Loop Break Stop**

**Screen # 14 - Control Action**

**Screen # 15 - Control Mode**

**Screen # 16 - Auto Tune**

**Screen # 17 - Proportional Gain Setup**

**Screen # 18 - Integral Gain Setup**

**Screen # 19 - Derivative Rate Gain Setup**

**Screen # 20 - Power Rate Control**

**Screen # 21 - Run Time**

**Screen # 22 - Power Failure Control**

## PID Control Mode Setup:

### **Screen # 10 - Calibration Gateway**

- Screen will default to SKIP Calibration Setup.
- **WARNING:** Do not enter the calibration gateway unless you have the proper calibration equipment to calibrate the sensor inputs associated with this control. Changing calibration settings in the controller can cause errors in sensor temperature readings and operation of the control. For instructions on how to use the calibration functions, contact your instrument supplier.
- With SKIP selected, press the MENU key to advance to screen # 11.




### **Screen # 11 - Global Sensor Offset Calibration**

- Use the UP/DOWN arrow keys to change the offset value.
- The use of another temperature device is required to determine the correct offset needed.
- Adjusting this value is offsetting the sensor input temperature being displayed.
- When complete, press MENU key to advance to screen # 12.



### **Screen # 12 - Over Temperature Stop**

- Use UP/DOWN arrow keys to change the value.
- When sensor temperature goes above this value, the output device will be turned off.
- When complete, press MENU key to advance to screen # 13.

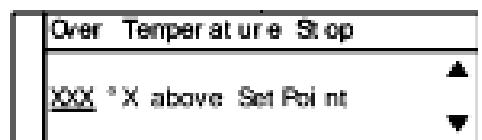

### **Screen # 13 - Loop Break Stop**

- Default value is ENABLED. Use UP/DOWN arrow keys to change the value.
- Loop Break Stop is a feature that will stop the process output while the controller is in the run mode. If the controller senses there is no change in temperature in a user set amount of time, the output will be turned off and error message will be displayed on the screen along with an audible alarm.
- Set to DISABLED if this function is not required.
- When complete, press MENU key to advance to screen # 14.



## PID Control Mode Setup:

### **Screen # 14 - Control Action**

- Use UP/DOWN arrow keys to change the value.
- Set for the process that is being performed: Heat or Cool
- When complete, press MENU key to advance to screen # 15.




### **Screen # 15 - Control Mode**

- Use UP/DOWN arrow keys to change the value.
- Default value is PID mode. (If different, select PID mode)
- When complete, press MENU key to advance to screen # 16.



### **Screen # 16 - Auto Tune**

- Default value is ENABLED. Use UP/DOWN arrow keys to toggle between ENABLED and DISABLED.
- Select ENABLED to use the Tune key on the front panel to activate the Auto Tune function. This function needs to remain ENABLED until the controller has been properly tuned to the user's particular application.
- When complete, press MENU key to advance to screen # 17.

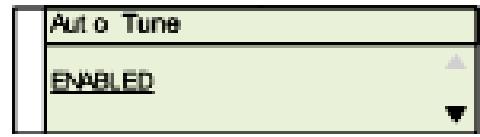

### **Screen # 17 - Proportional Gain Setup**

- Use UP/DOWN arrow keys to change the value.
- **WARNING:** Do not change these values unless you have experience in manual setup of PID (Proportional, Integral, and Derivative) of this controller. These values are derived from running the auto tune function. Altering the value after auto tune has been completed will affect the performance of the system.
- When complete, press MENU key to advance to screen # 19.



## PID Control Mode Setup:

### **Screen # 18 - Integral Gain Setup**

- Use UP/DOWN arrow keys to change the value.
- **WARNING:** Do not change these values unless you have experience in manual setup of PID (Proportional, Integral, and Derivative) of this controller. These values are derived from running the auto tune function. Altering the values after auto tune has been completed will affect the performance of the system.
- When complete, press MENU key to advance to screen # 21.



### **Screen # 19 - Derivative Rate Gain Setup**

- Use UP / DOWN arrow keys to change the value.
- **WARNING:** Do not change these values unless you have experience in manual setup of PID (Proportional, Integral, and Derivative) of this controller. These values are derived from running the auto tune function. Altering the value after auto tune has been completed will affect the performance of the system.
- When complete, press MENU key to advance to screen # 23.



## PID Control Mode Setup:


### **Screen # 20 - Power Output Control**

- Use UP/DOWN arrow keys to change the value.
- Default value is 100 percent.
- This feature allows the user to reduce the output power to the output heating device—useful in applications where temperature overshoot is occurring after auto tune has been completed.
- Experimenting with this value will be necessary because every process setup is different.
- When complete, press MENU key to advance to screen # 24.



### **Screen # 21 - Run Time**

- Use UP/DOWN arrow keys to change the value.
- Use SELECT key to toggle between the HR and MIN fields.
- Run Time is a safety feature while the control is in the ON/OFF or PID mode. The user can set a timer to have the output turned OFF if the time expires.
- When complete, press MENU key to advance to screen # 25.

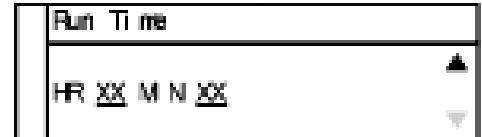

### **Screen # 22 - Power Failure Control**

- Use UP/DOWN arrow keys to change the value.
- Default value is STOP:

*STOP* — If the controller loses power while in the run mode, it will not resume the process once the power has been restored.

*RESUME* — If the controller loses power while in the run mode, it will resume the operating process once the power has been restored.

- When complete, press MENU key to advance to screen # 26.




### **Screen # 23 - Advanced Menu Exit**

- Setup is complete.
- Automatically exit to the main operation screen.

## **ON/OFF Control Mode Setup:**


### **Screen # 1 - Selecting Sensor Type**

- The TC9100 controller is set to thermocouple.
- Press MENU key to advance to next screen.

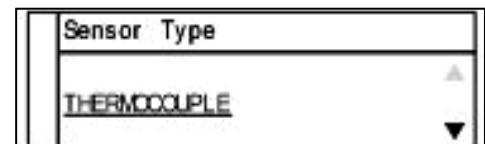

### **Screen # 2 - Selecting Thermocouple Type**

- Thermocouple is preselected on screen # 1.
- Use the UP/DOWN arrow keys to select the desired thermocouple type: J, K, N, R, S, T, B, or E.
- Press MENU key to advance to screen # 3 after selection has been made.

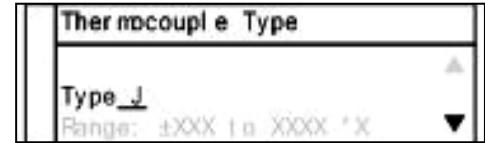

### **Screen # 3 - Selecting Temperature Scale**

- Use the UP/DOWN keys to select the desired temperature scale: Celsius °C, Fahrenheit °F, Kelvin K, Reaumur °Ré, or Rankine °Ra.
- Press MENU key to advance to screen # 4 after selection has been made.



## ON/OFF Control Mode Setup:

### Screen # 4 - Selecting Alarm Setting

- Use the UP/DOWN arrow keys to toggle between Auto Reset, Manual Reset, and Off.
- Press MENU key to advance to next screen:
  - If Auto or Manual is selected, the controller will advance to screen # 5.
  - If OFF is selected, the controller will advance to screen # 9.



### Screen # 5 - Selecting Alarm Mode

- Use the UP/DOWN arrow keys to select alarm mode.
- Selectable alarm modes:
  - **Process High:** The alarm will be activated if the temperature rises above the user set alarm value.
  - **Process Low:** The alarm will be activated if the temperature goes below the user set alarm value.
  - **Process High/Low:** The alarm will be activated if the temperature goes above or below the high and low temperature levels set by user.
- Press the MENU key to advance to screen # 6 after selecting alarm mode.



## **ON/OFF Control Mode Setup:**

### **Screen # 6 - Setting Alarm Mode Variables**

- This screen reflects the variable settings for the selected alarm mode from screen # 5.

#### **-Set Point—Process High**

- Use UP/DOWN arrow keys to adjust the temperature value.
- When complete, press MENU key to advance to screen # 7.

Process: High
HIGH <u>XXXX_X</u> °X

#### **- Set Point—Process Low**

- Use UP/DOWN arrow keys to adjust the temperature value.
- When complete, press MENU key to advance to screen # 7.

Process: Low
LOW <u>XXXX_X</u> °X

#### **- Set Point—Process High/Low**

- Use UP/DOWN arrow keys to adjust the temperature value.
- Press the SELECT key to toggle between High and Low.  
There will be a line below the active field.
- When complete, press MENU key to advance to screen # 7.

Process: High/ Low
High: <u>XXXX_X</u> °X
Low: <u>XXXX_X</u> °X

## **ON/OFF Control Mode Setup:**

### **Screen # 7 - Setting Hysteresis Alarm**

- Use the UP/DOWN arrow keys to adjust value.
- The user-defined value when the alarm will exit an alarm condition. **Example:** The user has a Process High alarm programmed with a value of 150°C and has set the Alarm Hysteresis of 1°C. The alarm has been activated after the temperature reached 160°C. When temperature reaches 149°C, the alarm condition will not be active.
- When complete, press MENU key to advance to screen # 8.



### **Screen # 8 - Setting Audible Alarm**

- Use UP/DOWN arrow keys to change value to either ON audible alarm or OFF audible alarm.
- When complete, press MENU key to advance to screen # 9.



### **Screen # 9 - Advanced Menu Gateway**

- Use UP/DOWN arrow keys to change selection to ENTER.
- When complete, press MENU key to advance to screen # 10.
- The following screens are in the advance portion of the setup menu:



**Screen # 10 - Calibration Gateway**

**Screen # 11 - Global Sensor Offset**

**Screen # 12 - Over Temperature Stop**

**Screen # 13 - Loop Break Stop**

**Screen # 14 - Control Action**

**Screen # 15 - Control Mode**

**Screen # 16 - On/Off Control**

**Screen # 17 - Power Output Control**

**Screen # 18 - Run Time**

**Screen # 19 - Power Failure Control**

## ON/OFF Control Mode Setup:

### **Screen # 10 - Calibration Gateway**

- Screen will default to SKIP Calibration Setup.
- **WARNING:** Do not enter the calibration gateway unless you have the proper calibration equipment to calibrate the sensor inputs associated with this controller. Changing calibration settings in the control can cause errors in sensor temperature readings and operation of the control. For instructions on how to use the calibration functions, contact your instrument supplier.
- With SKIP selected, press the MENU key to advance to screen # 11.




### **Screen # 11 - Global Sensor Offset Calibration**

- Use the UP/DOWN arrow keys to change the offset value.
- The use of another temperature device is required to determine the correct offset needed.
- Adjusting this value is offsetting the sensor input temperature being displayed.
- When complete, press MENU key to advance to screen # 12.



### **Screen # 12 - Over Temperature Stop**

- Use the UP/DOWN arrow keys to change the value.
- When sensor temperature goes above this value, the output device will be turned off.
- When complete, press MENU key to advance to screen # 13.

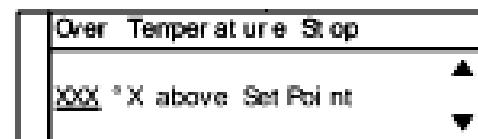

### **Screen # 13 - Loop Break Stop**

- Default value is ENABLED. Use the UP/DOWN arrow keys to change the value.
- Loop Break Stop is a feature that will stop the process output while the control is in the run mode. If the control senses there is no change in temperature in a user set amount of time the output will be turned off and error will be displayed on the screen along with a audible alarm.
- Set to DISABLED if this function is not required.
- When complete, press MENU key to advance to screen # 14.



## **ON/OFF Control Mode Setup:**


### **Screen # 14 - Control Action**

- Use the UP/DOWN arrow keys to change the value from Heat to Cool.
- Set for the particular process that is being performed.
- When complete, press MENU key to advance to screen # 15.



### **Screen # 15 - Control Mode**

- Use UP/DOWN arrow keys to change the value from the default mode of PID to On/Off.
- When complete, press MENU key to advance to screen # 16.

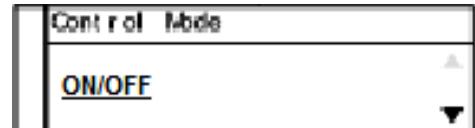


### **Screen # 16 - ON/OFF Control**

- Use the UP/DOWN arrow keys to adjust value.
- Cycle time is the rate that the output cycles on and off. The recommended time is 1 second.
- If a mechanical relay is being used from the output, it is recommended that the time be increased to more than 1 second. Mechanical relays are slower than solid-state relays and require more time to operate correctly. Damage to the relay and control can occur if not set correctly.
- When complete, press MENU key to advance to screen # 17.



### **Screen # 17 - Power Output Control**


- Use UP/DOWN arrow keys to change the value.
- Default value is 100 percent.
- This feature allows the user to reduce the output power to the output heating device—useful in applications where temperature overshoot is occurring after Auto Tune has been completed.
- Experimenting with this value will be necessary because every process setup is different.
- When complete, press MENU key to advance to screen # 18.

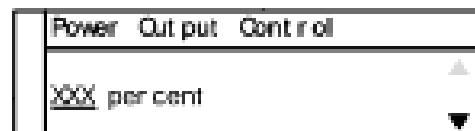

## **ON/OFF Control Mode Setup:**

### **Screen # 18 - Run Time**

- Use the UP/DOWN arrow keys to change the value.
- Use the SELECT key to toggle between HR and MIN fields.
- Run Time is a safety feature while the control is in the On/Off or PID mode. The user can set a timer to have the output turned OFF if the time expires.
- When complete, press MENU key to advance to screen # 19.

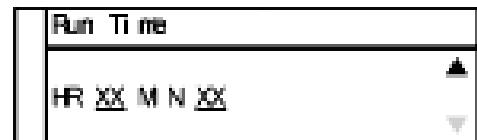

### **Screen # 19 - Power Failure Control**

- Use the UP/DOWN arrow keys to change the value.
- Default value is STOP:

*STOP* — If the controller loses power while in the run mode, it will not resume the process once the power has been restored.

*RESUME* — If the controller loses power while in the run mode, it will resume the operating process once the power has been restored.

- When complete, press MENU key to advance to screen # 20.



### **Screen # 20 - Advanced Menu Exit**

- Setup is complete.
- Automatically will exit to the main operation screen.

## Safety Precautions



**DANGER: DO NOT REMOVE COVER! HIGH VOLTAGE IS PRESENT IN THE CONTROLLER.** Contact supplier for service.



**DANGER: If high voltage is present on external temperature sensor from outside source, high voltage will be present at the control.**



**DANGER: Fire protection and control damage: Replace all fuses with the correct fuse replacement. Reference page 26 for model 89800-11 and page 27 for model 89800-12.**



**WARNING: Specifications for the power cord: see page 26 for model 89800-11 and page 27 for model 89800-12 for proper replacement cord. Additional input power cords for various countries are listed on page 32.**



**WARNING: Use of separate temperature limit control is recommended were a fault condition could occur and result in a fire or other hazardous condition.**

## **Specifications for TC9100 Controller — Model 89800-11**

**Power input:** 120 VAC  $\pm 10\%$ , 50/60 Hz  $\pm 3\%$ , 15 amp, 1800 watts max load

**Operating environment:** 32 to 77°F (0 to 25°C); 90% RH, noncondensing

**Maximum altitude:** 2187 yd (2000 m)

**Pollution degree:** 2 (normally only nonconductivity pollution occurs)

**Installation category II:** local level (connect to branch circuit and not directly to a main circuit,  
such as a fuse panel)

**Storage:** 32 to 140°F (0 to 60°C); 5 to 80% RH, noncondensing

**Fuse:** 250 volt, 15 amp rated (fast-acting)

**AC line cord:** SJT-14-3 14 AWG, 15 amp, 125 VAC, less than 9 ft (3 m) in length

**Heater/cooler output:** max voltage: 120 VAC  $\pm 10\%$ , 15 amp, 50/60 Hz, 1800 watts max load

**Process memory:** data retention upon power failure via nonvolatile memory

**Dimensions (W x H x D):** 8" x 3.75" x 9" (20.3 x 9.5 x 22.9 cm)

## **Specifications for TC9100 Controller — Model 89800-12**

**Power input:** 230 VAC  $\pm 10\%$ , 50/60 Hz  $\pm 3\%$ , 10 amp, 2300 watts max load

**Operating environment:** 32 to 77°F (0 to 25°C); 90% RH, noncondensing

**Maximum altitude:** 2187 yd (2000 m)

**Pollution degree:** 2 (normally only nonconductivity pollution occurs)

**Installation category II:** local level (connect to branch circuit and not directly to a main circuit,  
such as a fuse panel)

**Storage:** 32 to 140°F (0 to 60°C); 5 to 80% RH, noncondensing

**Fuse:** 250 volt, 10 amp rated (fast-acting)

**AC line cord:** SJT-14-3 14 AWG, 15 amp, 240 VAC, less than 9 ft (3 m) in length

**Heater/cooler output:** max voltage: 230 VAC  $\pm 10\%$ , 15 amp, 50/60 Hz  $\pm 3\%$ , 3450 watts max load

**Process memory:** data retention upon power failure via nonvolatile memory

**Dimensions (W x H x D):** 8" x 3.75" x 9" (20.3 x 9.5 x 22.9 cm)

## Specifications for Sensor Input

- Thermocouple (grounded or nongrounded)
- Automatic cold junction compensation and break protection for sensor

### Range

Type J	<b>-310 to 1832°F (-190 to 1000°C)</b>
Type K	<b>-328 to 2502°F (-200 to 1372°C)</b>
Type N	<b>-328 to 2372°F (-200 to 1300°C)</b>
Type R	<b>32 to 3214°F (0 to 1768°C)</b>
Type S	<b>32 to 3214°F (0 to 1768°C)</b>
Type T	<b>-200 to 752°F (-200 to 400°C)</b>
Type B	<b>392 to 3272°F (200 to 1800°C)</b>
Type E	<b>-328 to 1832°F (-200 to 1000°C)</b>

### Sensor accuracy


#### Calibration accuracy

Types J, K, T, E, N:  $\pm 0.1\%$  of span or  $\pm 1^\circ\text{C}$


Types B, R, S:  $\pm 0.2\%$  of span

Accuracy span is 1000°F (540°C) minimum

# Screen Flow Charts

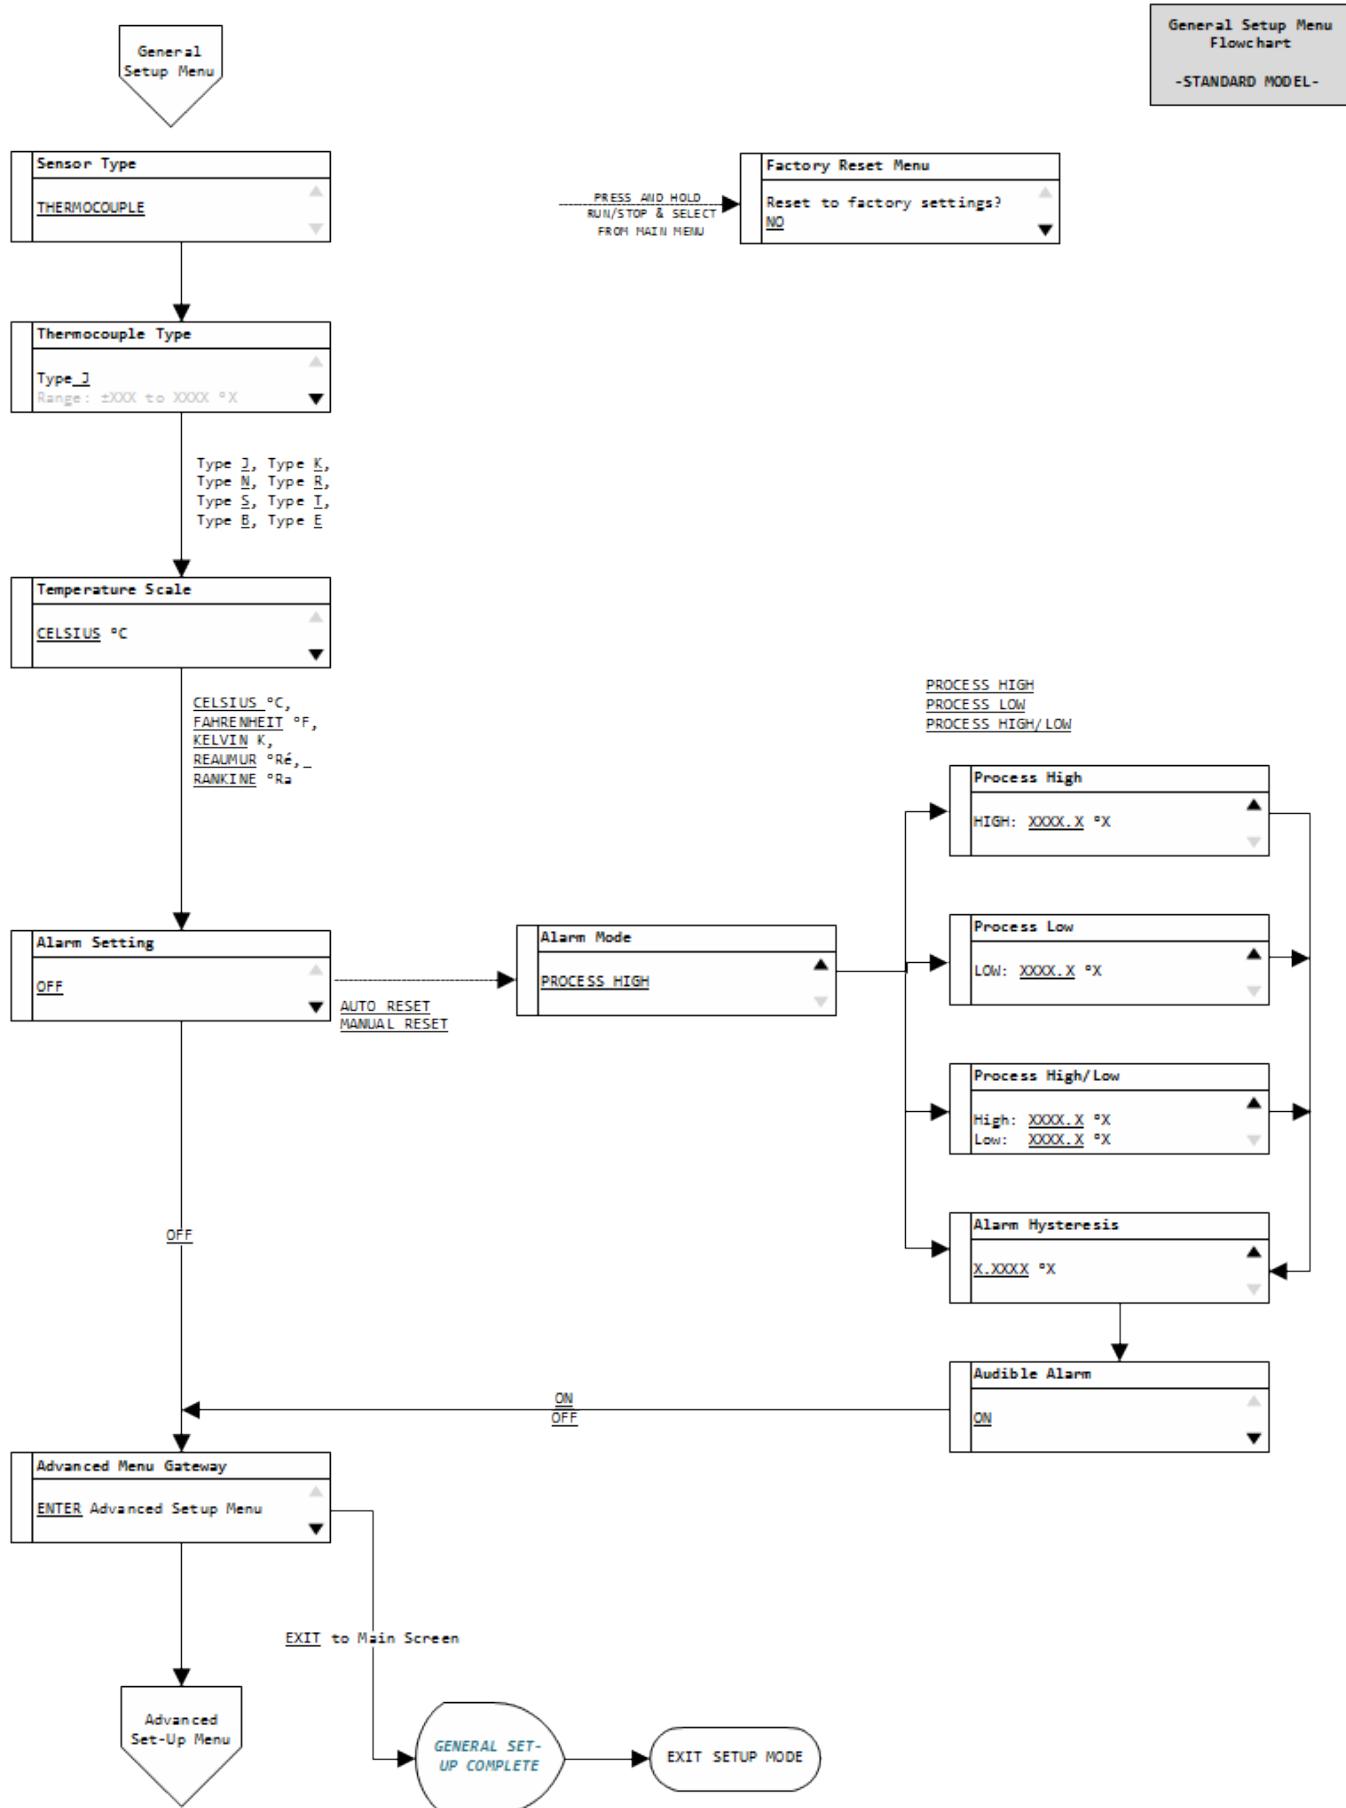

# Screen Flow Charts

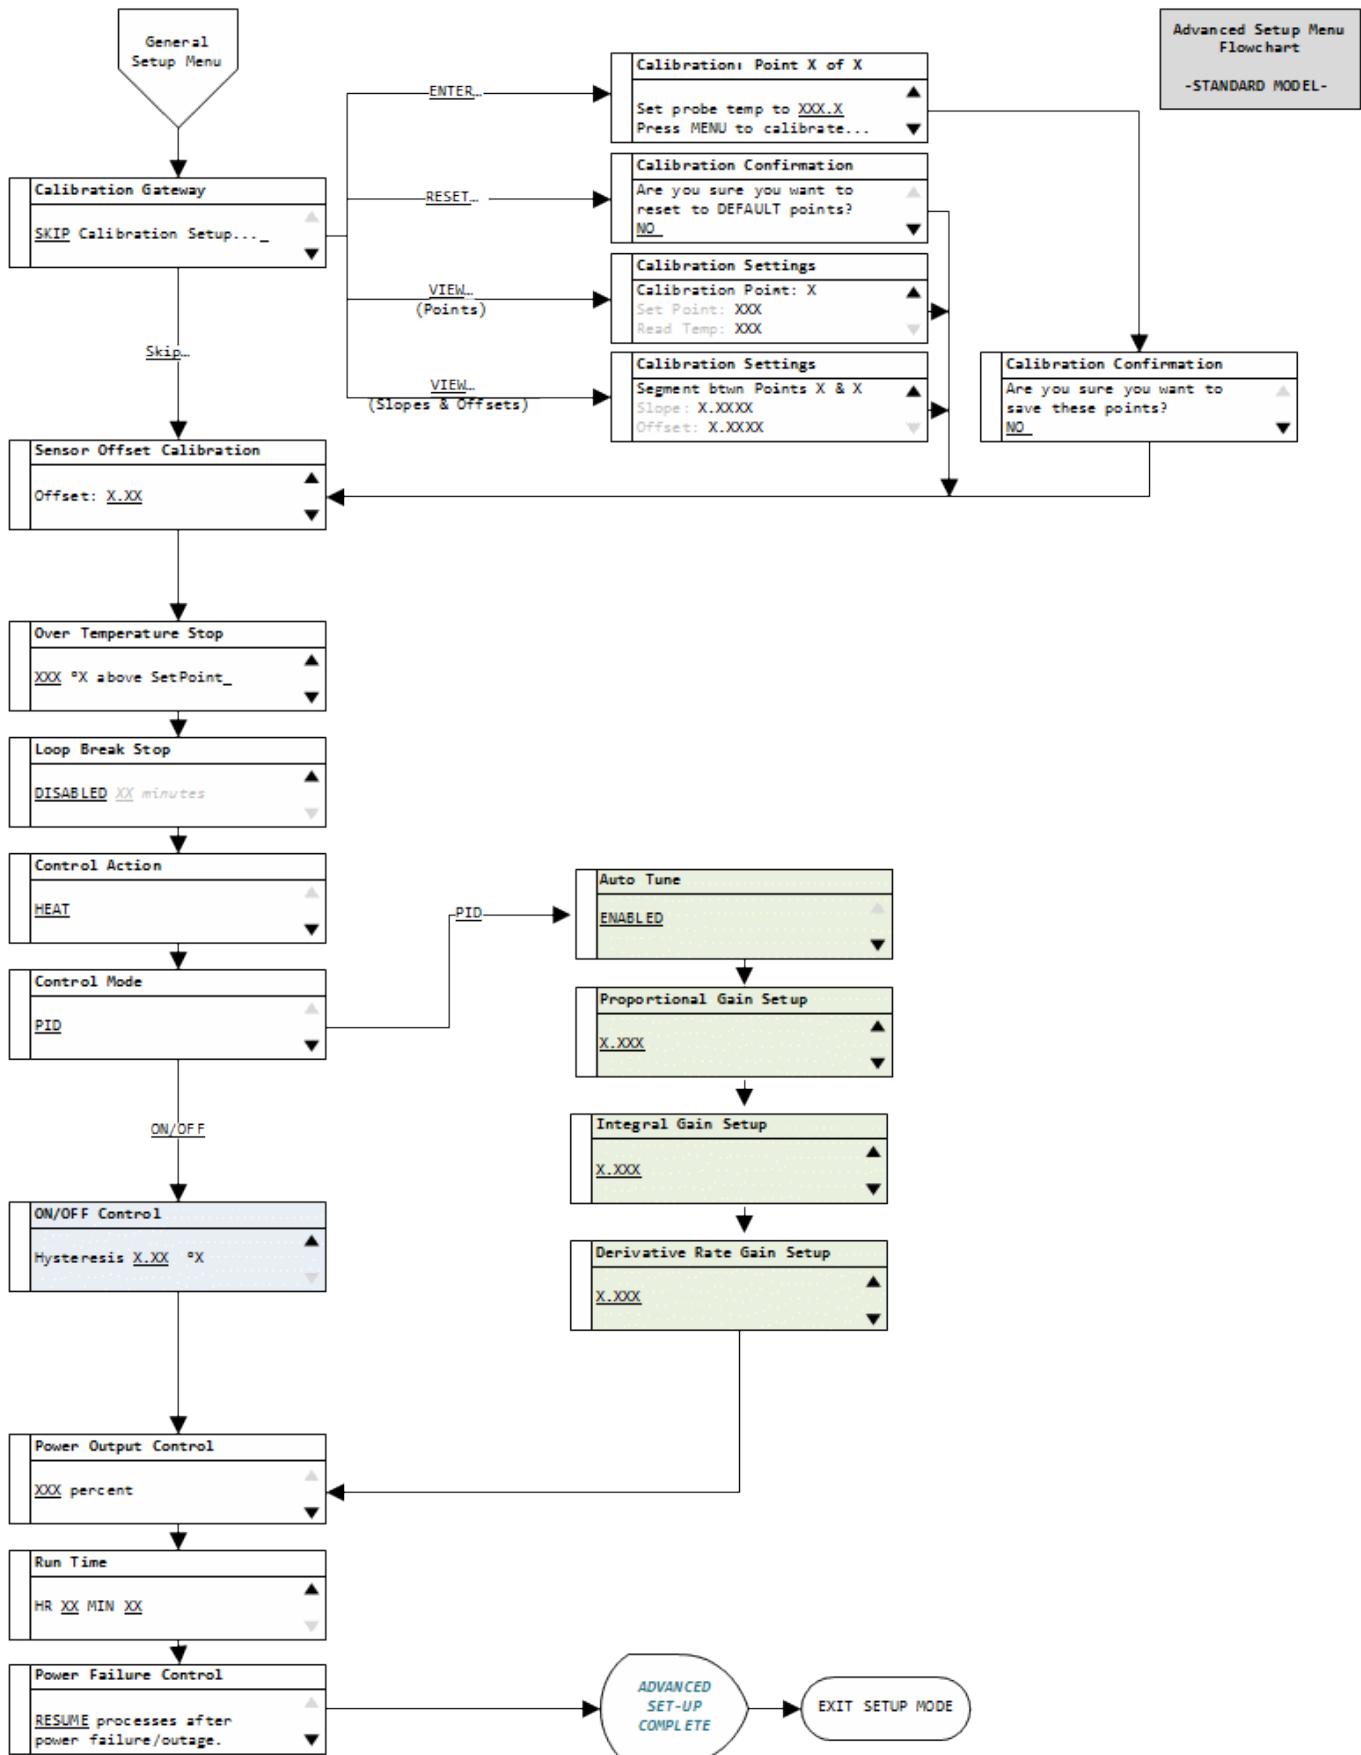

## Ferrite Clip Installation




Example picture Digi-Sense Temperature Controller TC9100 Model 89800-13

## Alternative Power Cords — for Various Countries









A detachable cord/plug set is automatically included with both models of the temperature controller:

- Model 89800-11 includes a US 120 VAC plug
- Model 89800-12 includes a US 220 VAC plug

Below is a ordering table for the available cord/plug sets. Cord/plug sets feature a country-specific male plug on one end and an IEC 320 female plug on the other end. Order a cord/plug set to replace a lost or damaged set or to use your temperature controller in another country.



IEC 320 socket


Illustration	Country	Catalog number
	US Standard	50001-68
	Australia, Japan	50001-60
	Denmark	50001-62
	India	50001-64
	Israel	50001-69
	Europe	50001-70
	England	50001-72
	Switzerland	50001-74
	Italy	50001-76
	US (NEMA)	50001-78

## Output Cord Adapters — for Various Countries

A detachable cord set is not included with the temperature controller:

- Model 89800-11 includes a US 120 VAC female plug
- Model 89800-12 includes a IEC 60320 C19, 230 VAC female plug

Below is a ordering table for the available cord sets. Cord sets feature a country-specific female plug on one end and an IEC 360320 C19 male plug on the other end that will plug into the controller.. Order a cord set to use your heating or cooling devices with your 230 VAC temperature controller in another country. Each cord set is 12 in ((30.5 cm) in length.



IEC 60320 C19

Illustration	Country	Catalog number
An illustration showing a male IEC 60320 C19 plug on the left and a female Australia/Japan plug on the right. The Australia/Japan plug has two round pins on the top row and one round pin on the bottom row.	Australia, Japan	80800-24
An illustration showing a male IEC 60320 C19 plug on the left and a female Denmark plug on the right. The Denmark plug has two round pins on the top row and one central pin on the bottom row.	Denmark	80800-21
An illustration showing a male IEC 60320 C19 plug on the left and a female India plug on the right. The India plug has two round pins on the top row and one central pin on the bottom row.	India	80800-23
An illustration showing a male IEC 60320 C19 plug on the left and a female Israel plug on the right. The Israel plug has three round pins on the top row and one central pin on the bottom row.	Israel	80800-28
An illustration showing a male IEC 60320 C19 plug on the left and a female Europe plug on the right. The Europe plug has two round pins on the top row and one central pin on the bottom row.	Europe	89800-19
An illustration showing a male IEC 60320 C19 plug on the left and a female England plug on the right. The England plug has three round pins on the top row and one central pin on the bottom row.	England	89800-22
An illustration showing a male IEC 60320 C19 plug on the left and a female Switzerland plug on the right. The Switzerland plug has two round pins on the top row and one central pin on the bottom row.	Switzerland	80800-26
An illustration showing a male IEC 60320 C19 plug on the left and a female Italy plug on the right. The Italy plug has two round pins on the top row and one central pin on the bottom row.	Italy	80800-27
An illustration showing a male IEC 60320 C19 plug on the left and a female US (NEMA) plug on the right. The US (NEMA) plug has two round pins on the top row and one central pin on the bottom row.	US (NEMA)	80800-29

## CE Approval

*Conforms to the following Product Specifications:*

EMC: EC Directive 204/108/EC

Using the following: EN 61326-1-2006

EN 55011: 2009 ISM RADIO FREQUENCY EQUIPMENT, CLASS B

EN 61000-3-2:2006 (IEC 61000-3-2: 2005) HARMONICS

EN 61000-3-3:2008 (IEC 61000-3-3:2008) FLICKER

Immunity Test:

EN 61000-4-2:2001-4 ESD

EN 61000-4-3:2006-02 RADIATED RF SUSCEPTIBILITY

EN 61000-4-4:2004-07 ELECTRICAL FAST TRANSIENT / BURST

EN 61000-4-5:2001-04 SURGE

EN 61000-4-6:2004-11 RF CONDUCTED SUSCEPTIBILITY, COMMON MODE

EN 61000-4-11:2004-03 VOLTAGE DIPS AND INTERRUPTIONS

Safety: 2006/95/EC using EN61010-1

## UL File E207546, Vol. 1

<b>Standard:</b>	UL 61010-1, 3rd Edition, 2012-04-17 (ELECTRICAL EQUIPMENT FOR MEASUREMENT, CONTROL, AND LABORATORY USE - Part 1: General Requirements) CAN/CSA-C22.2 No. 61010-1, 3rd Edition, 2012-04, (ELECTRICAL EQUIPMENT FOR MEASUREMENT, CONTROL, AND LABORATORY USE - Part 1: General Requirements)
<b>Certification Type:</b>	Listing
<b>CCN:</b>	OGTK, OGTK7 (Laboratory Use Electrical Equipment)

## **Maintenance**

- Simple preventive maintenance steps include keeping the controller clean. Protect it from overload, excessive dirt, oil and corrosion.
- Cleaning: If cleaning is necessary, use only a damp cloth with water only. Wipe only the exterior of the control chassis.

CATALOG NUMBERS **89800-11 and 89800-12**

SERIAL NUMBER \_\_\_\_\_

DATE OF PURCHASE \_\_\_\_\_